

FIG 3

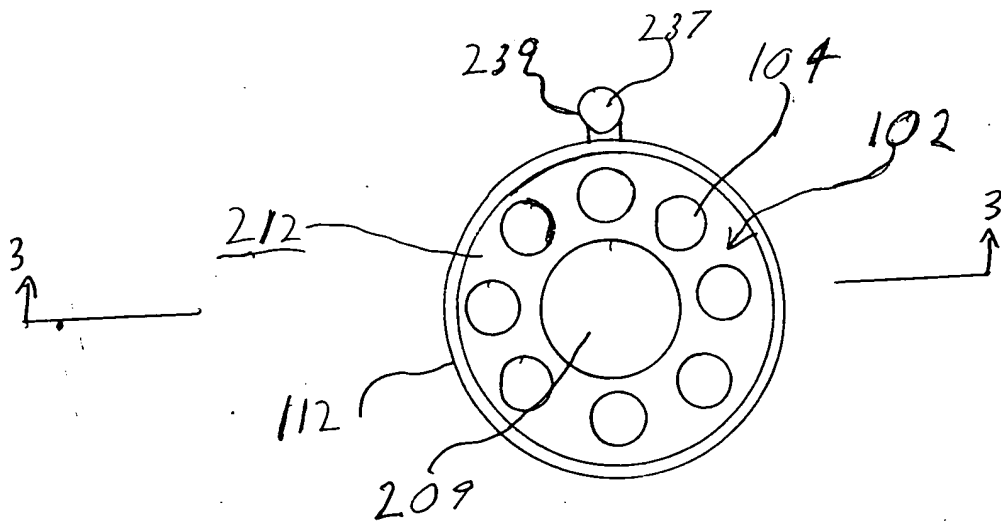


FIG 4

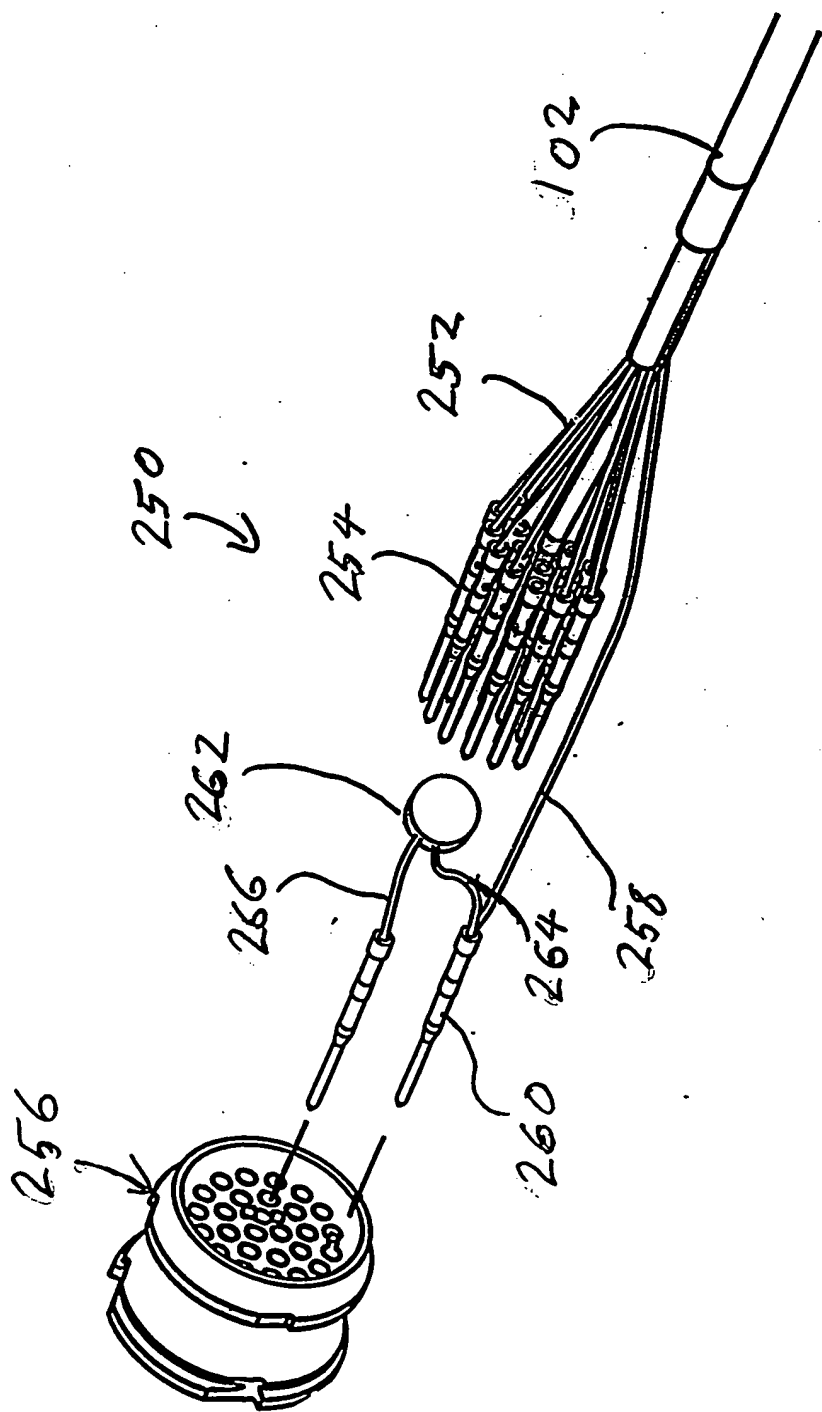


FIG. 5

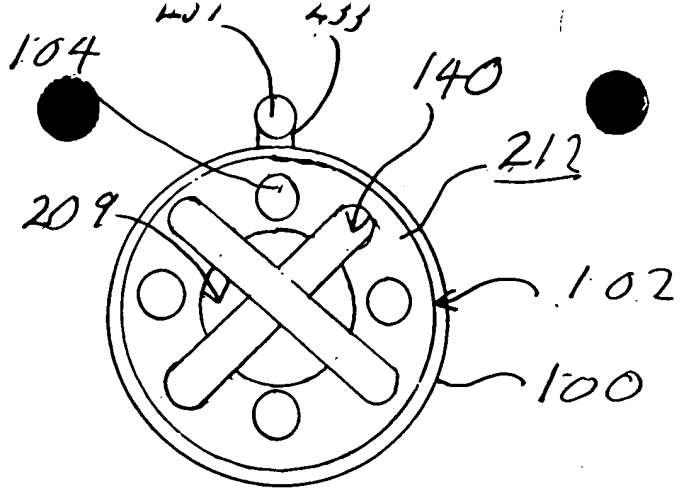


FIG. 6

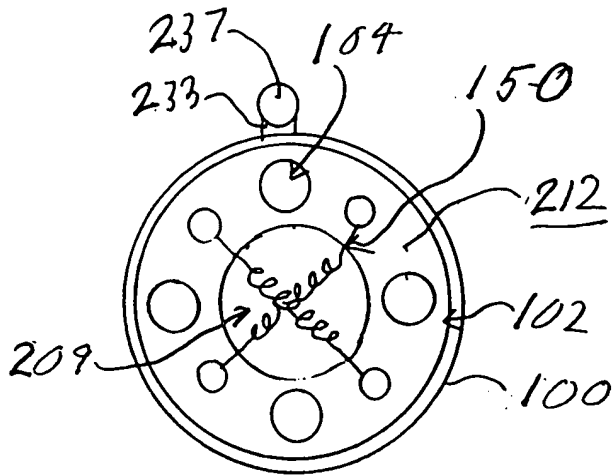


FIG. 7

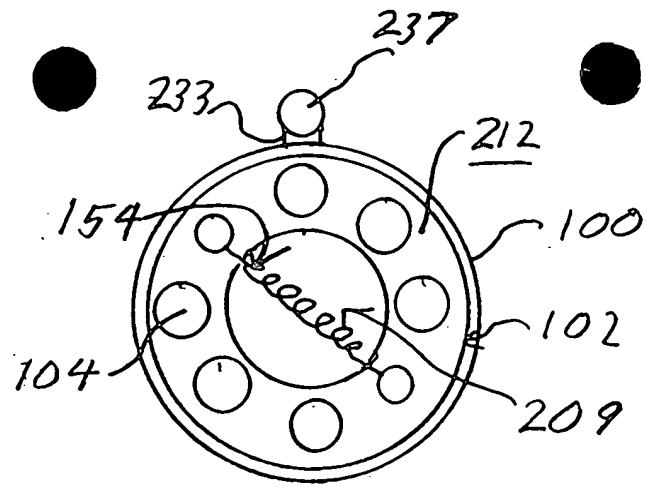


FIG. 8


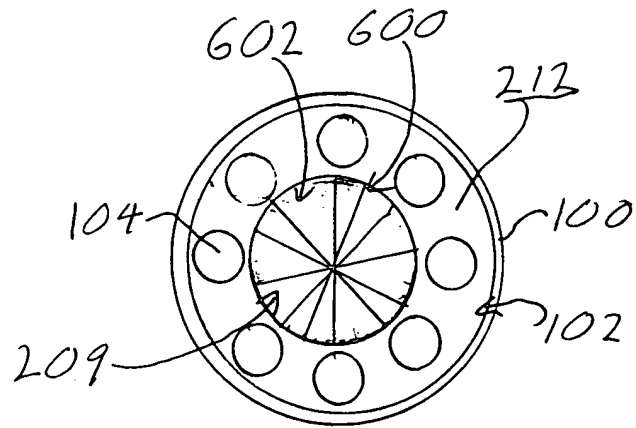


FIG. 9



90 ↗

F1610

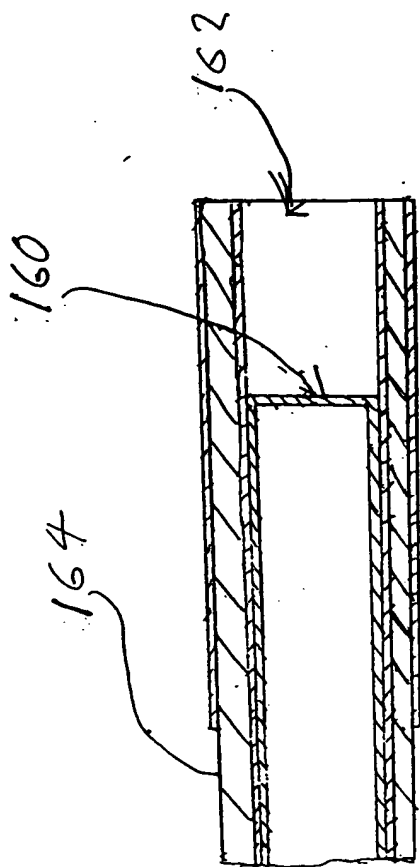

004220" 2122F550

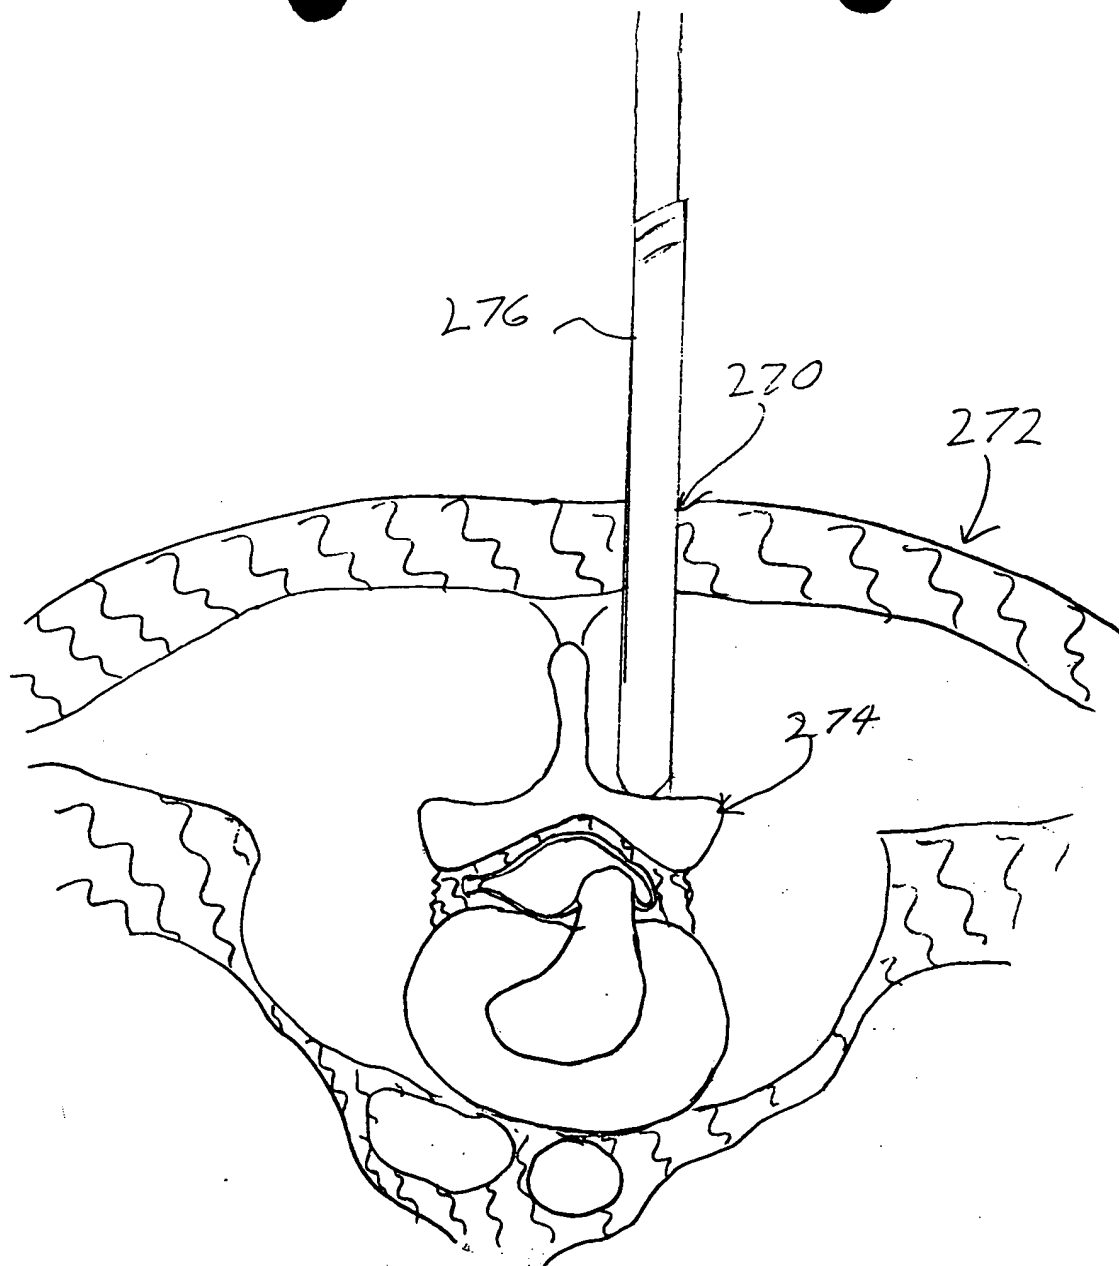


FIG. 12

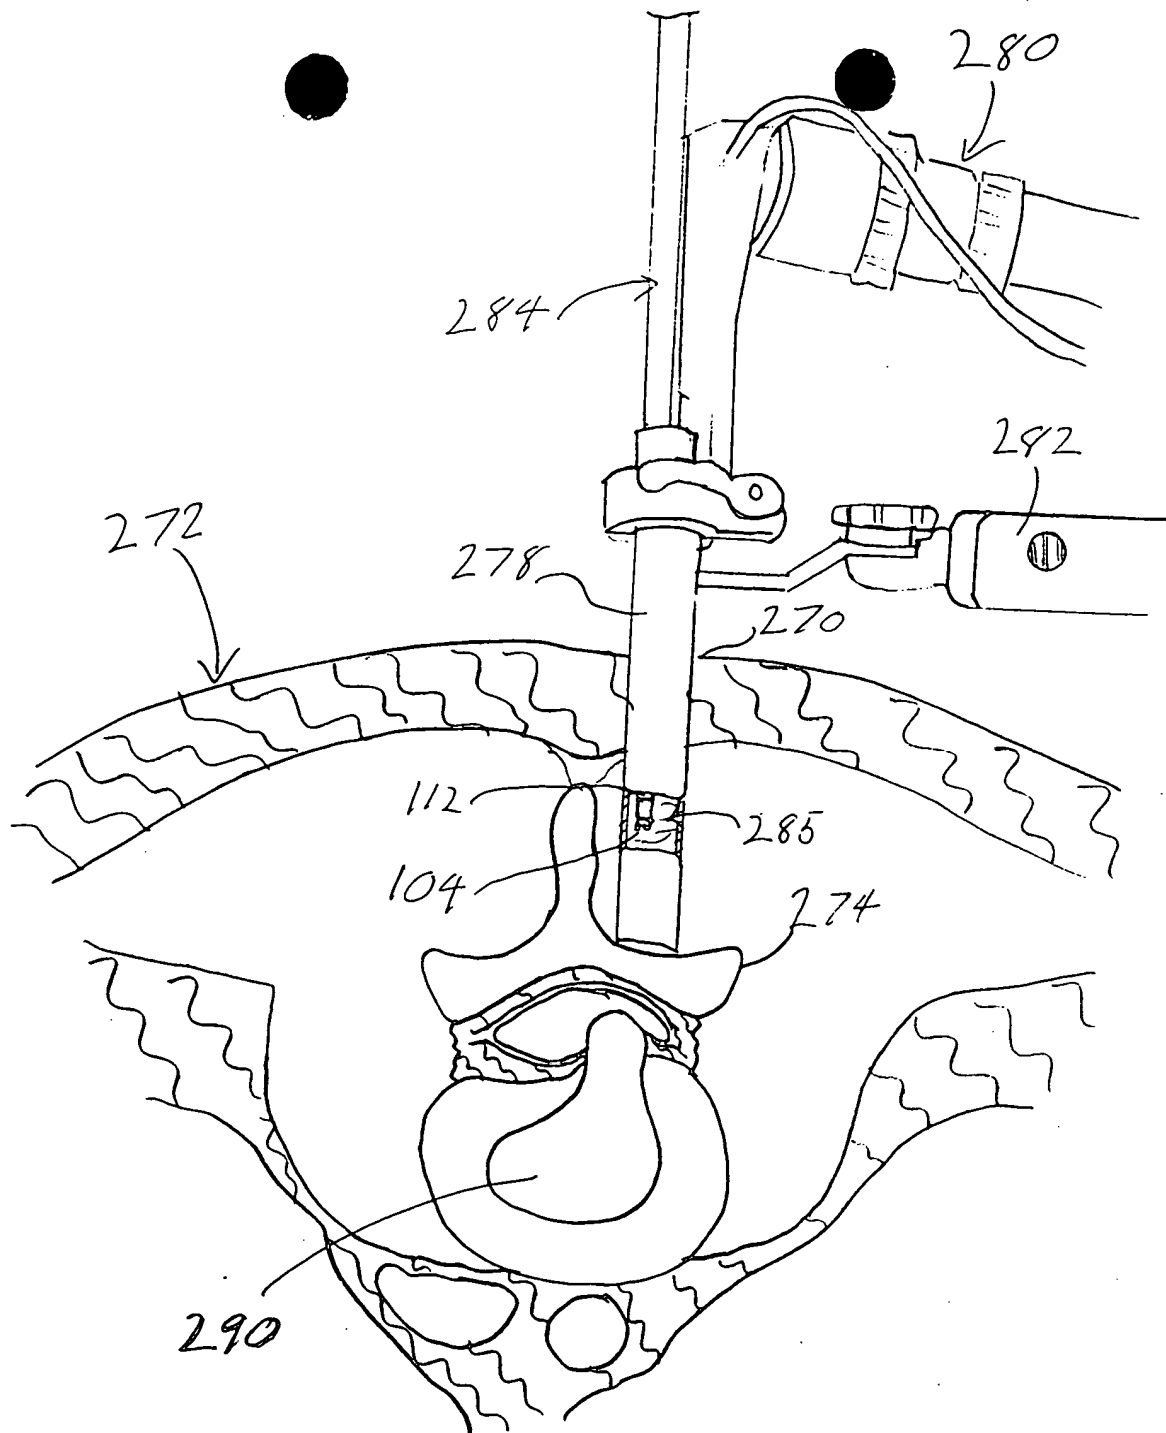


FIG 13.

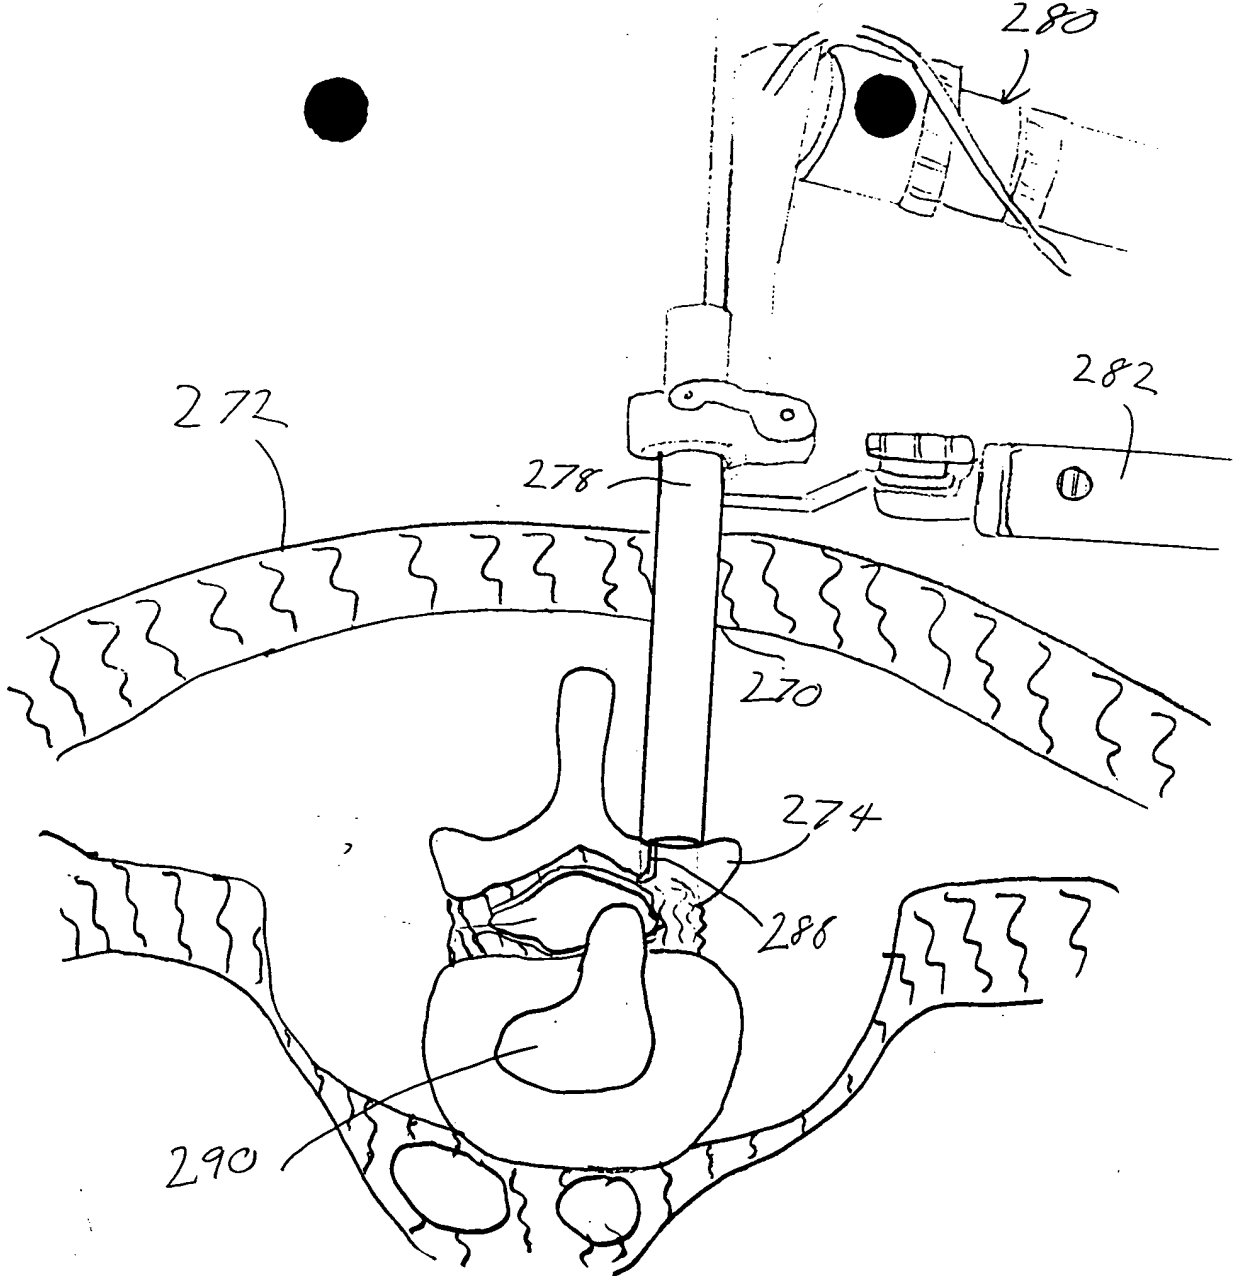


FIG. 14

00000-2122500

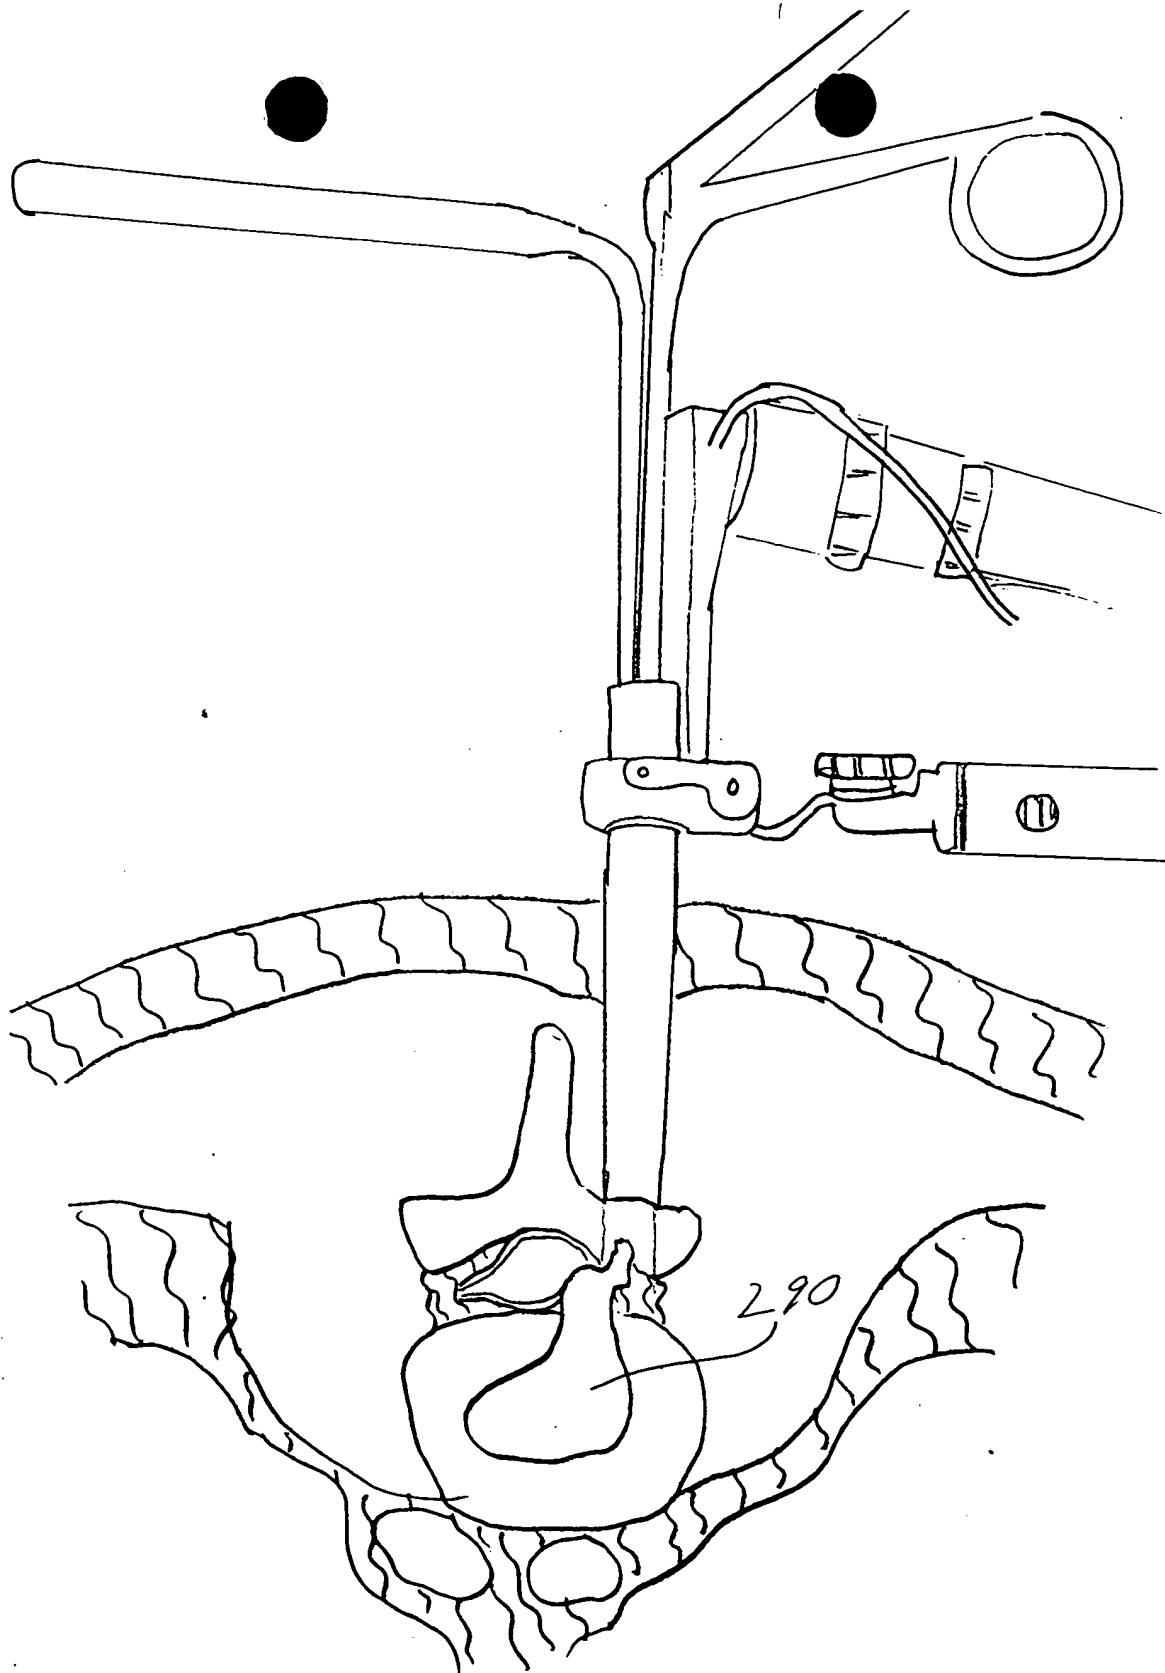


FIG. 15

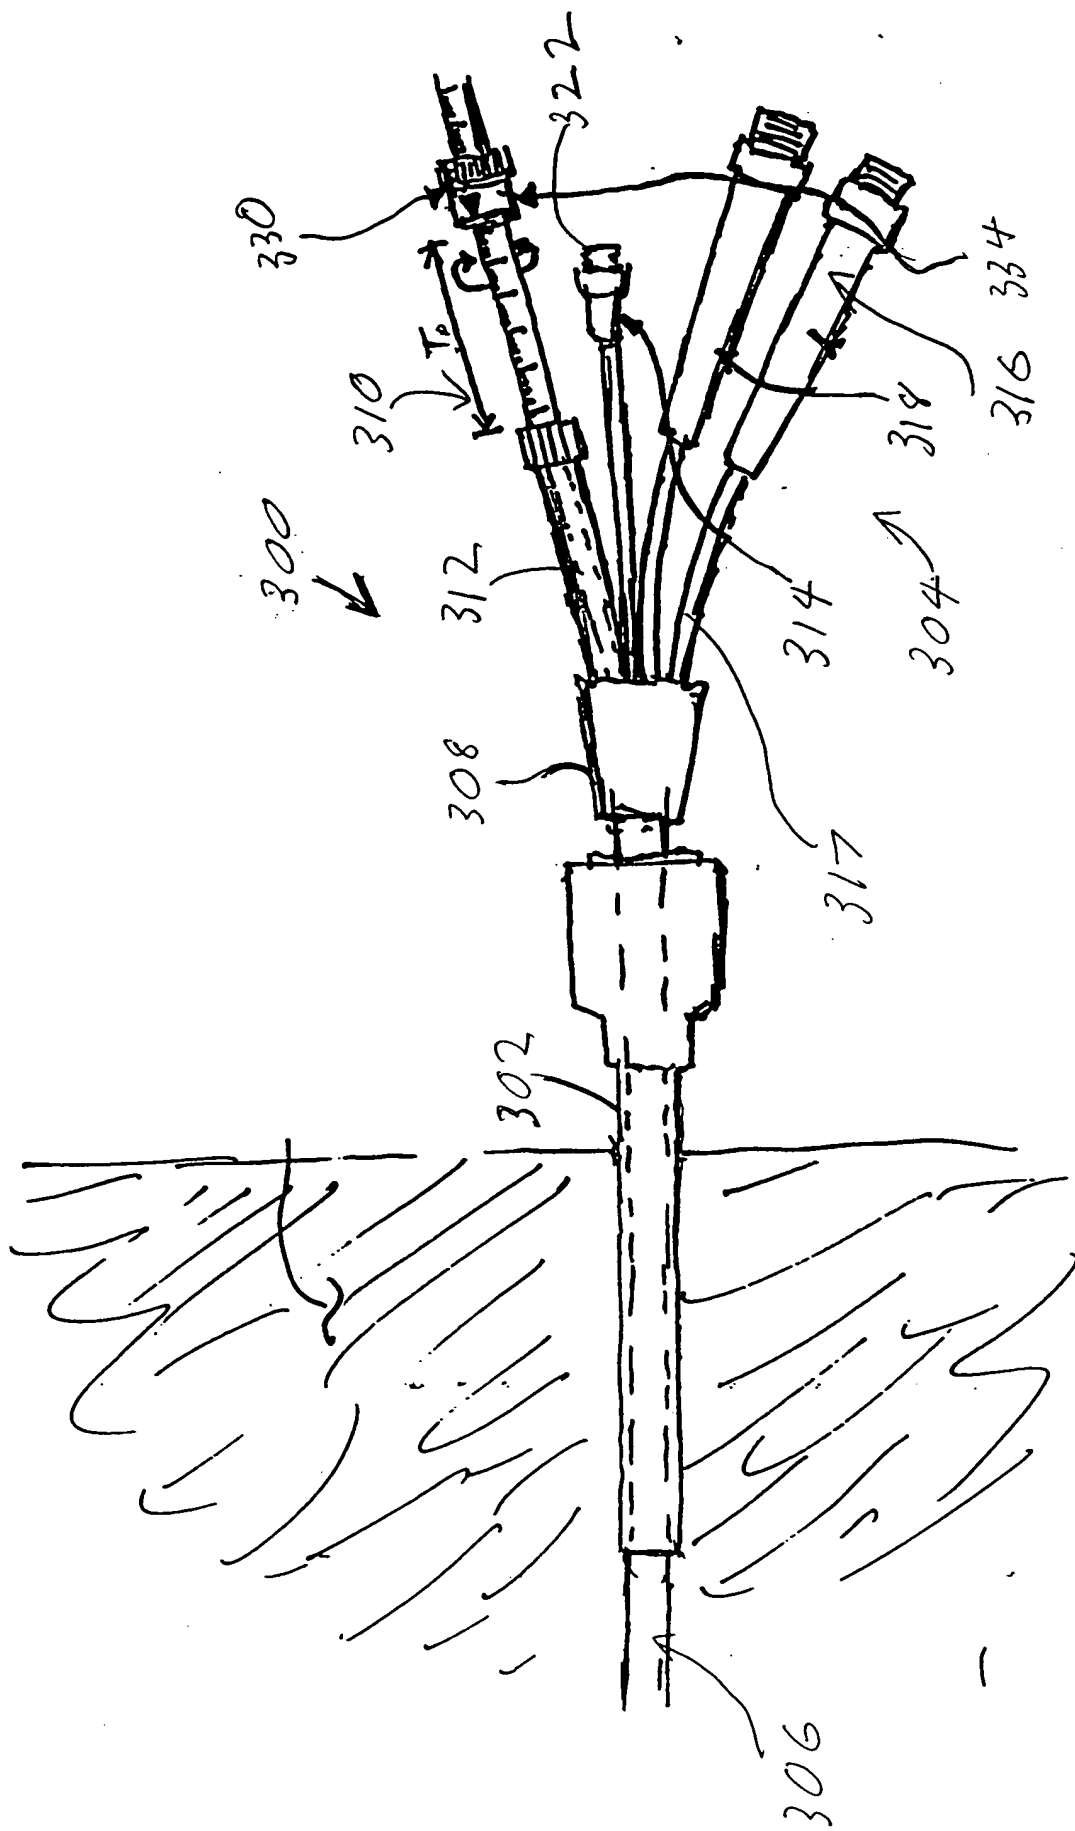


FIG. 16

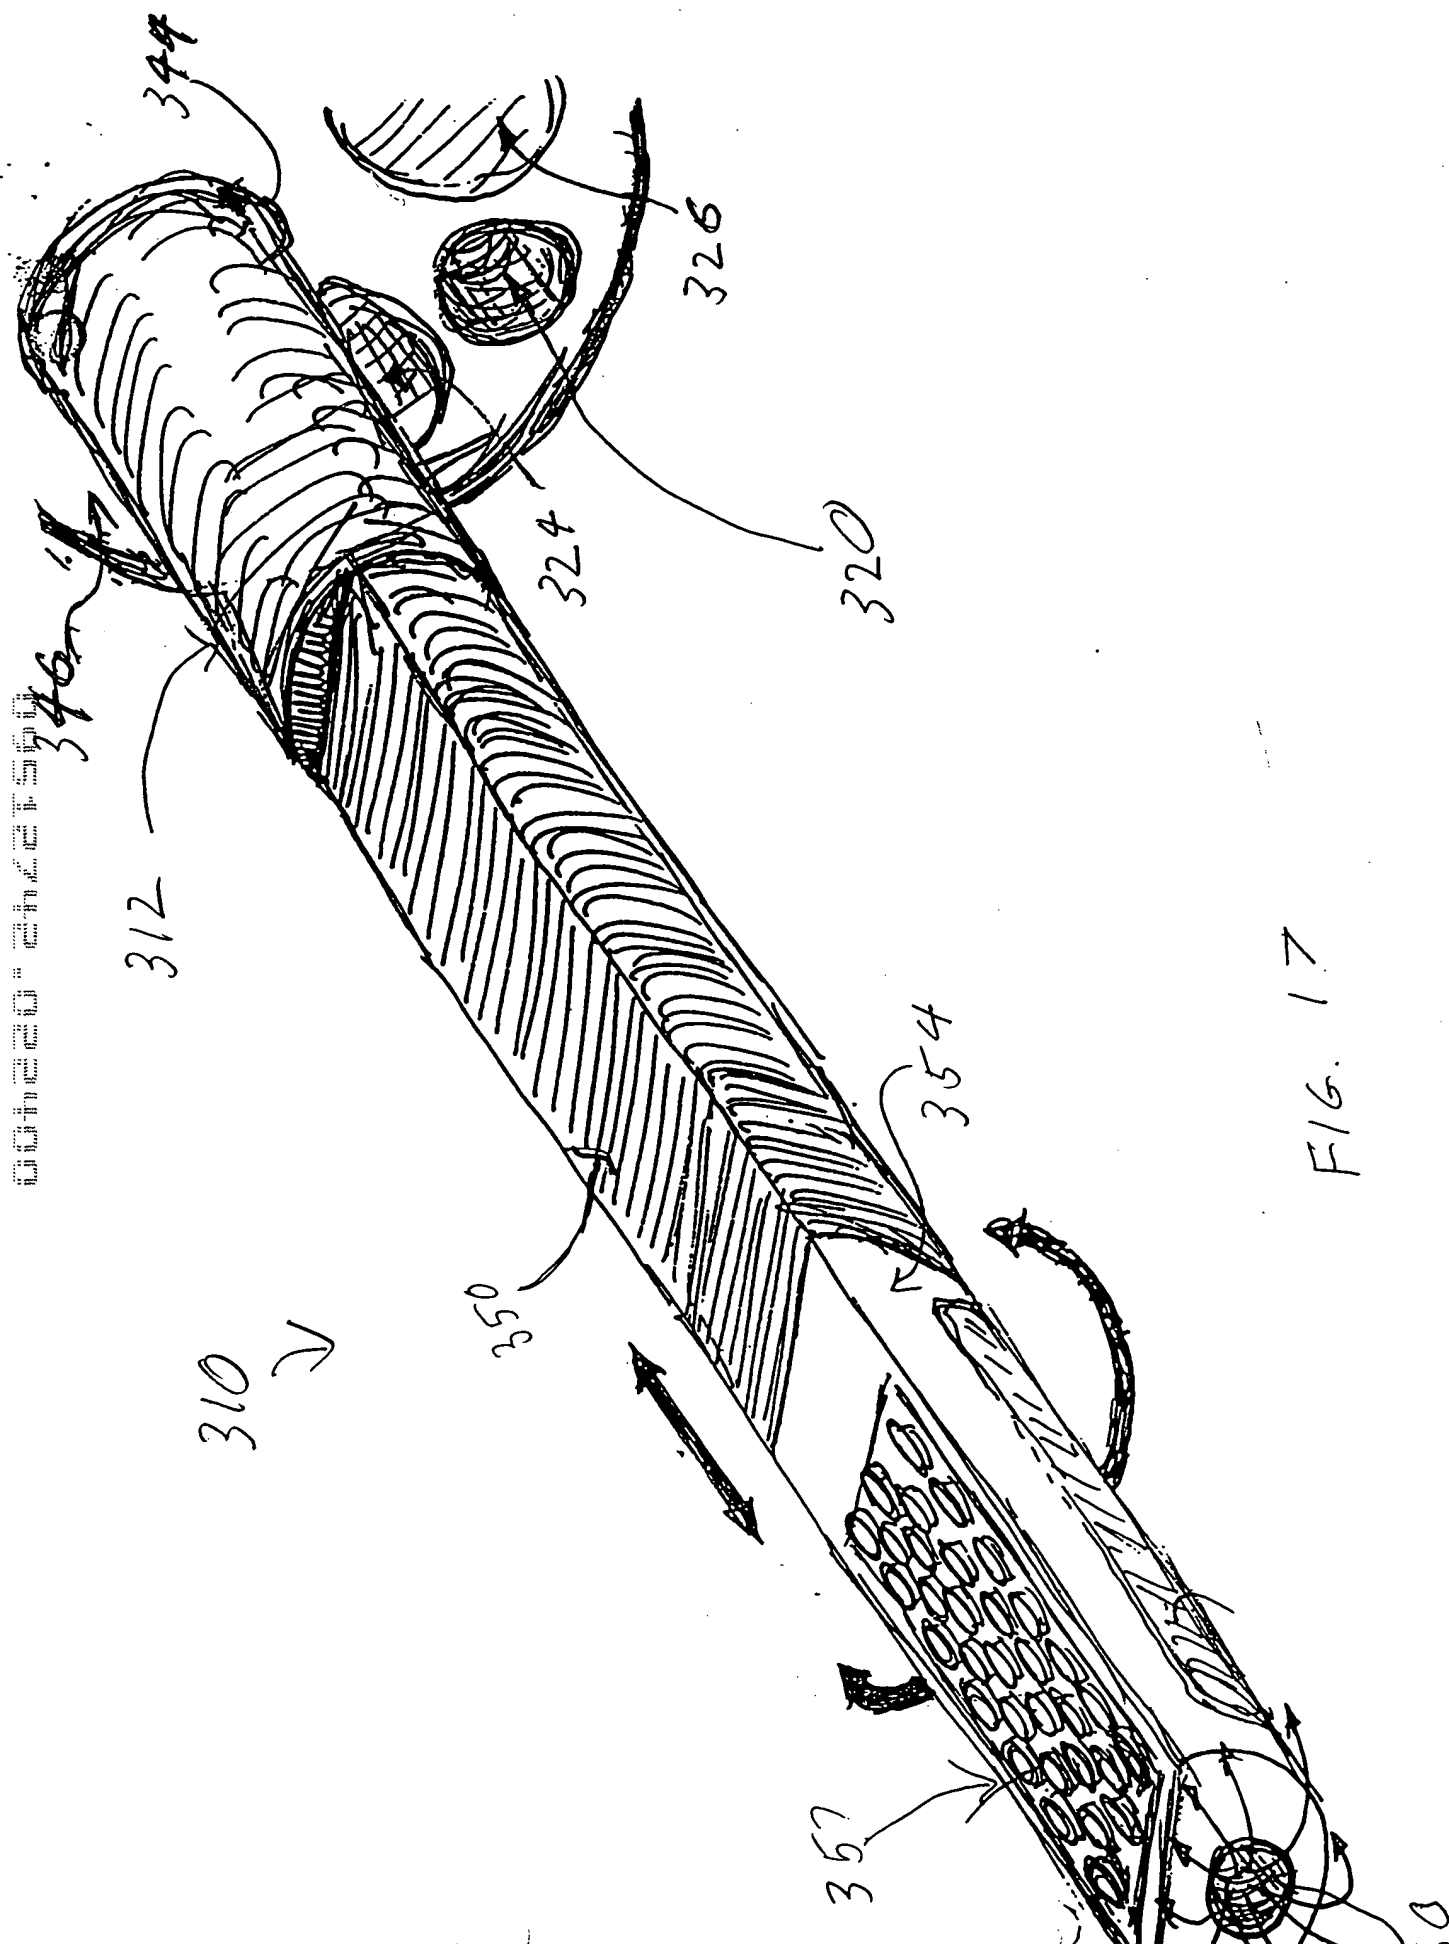


FIG. 17

004220-2422560

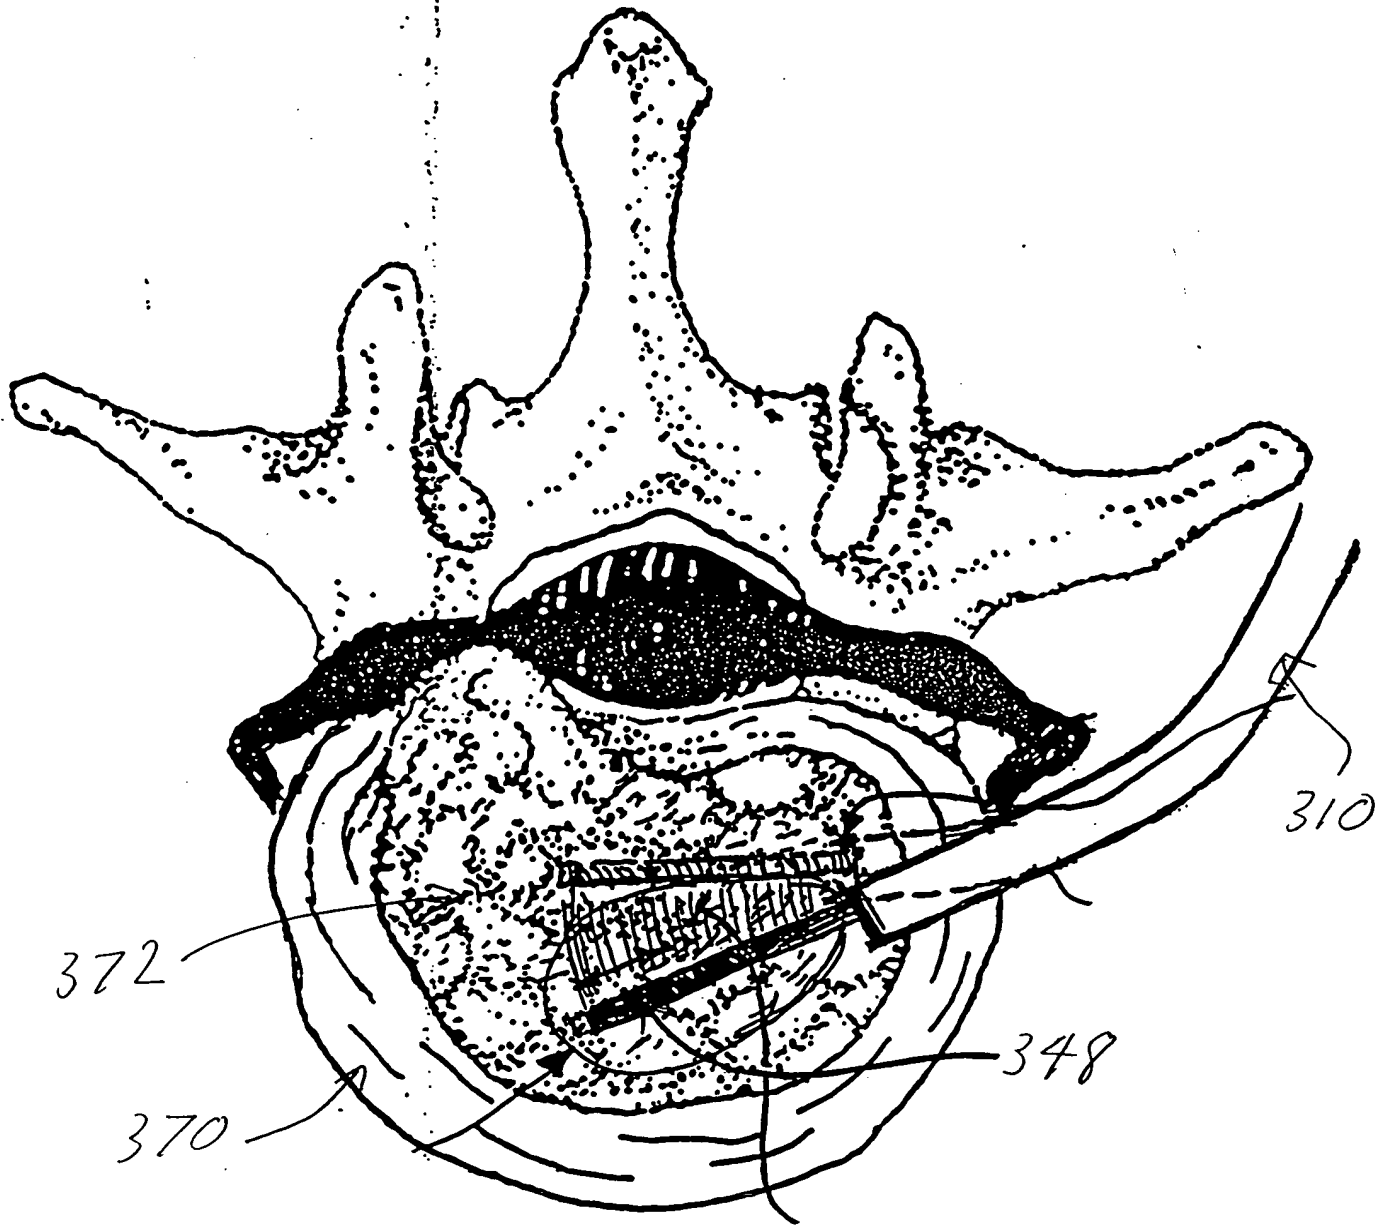


FIG. 18

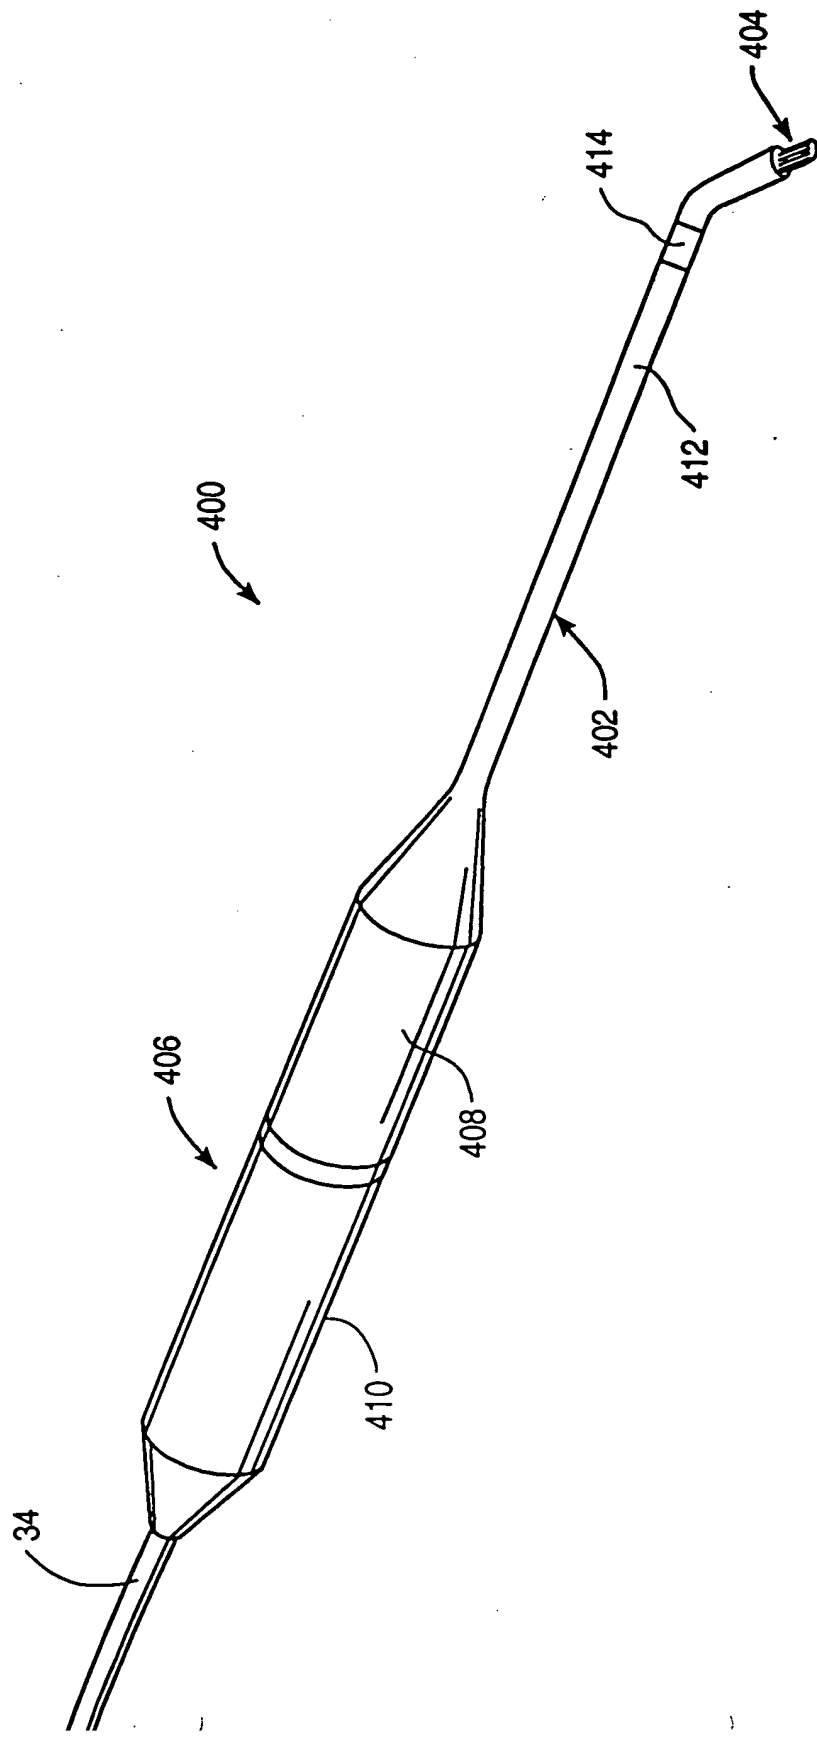


FIG. 19

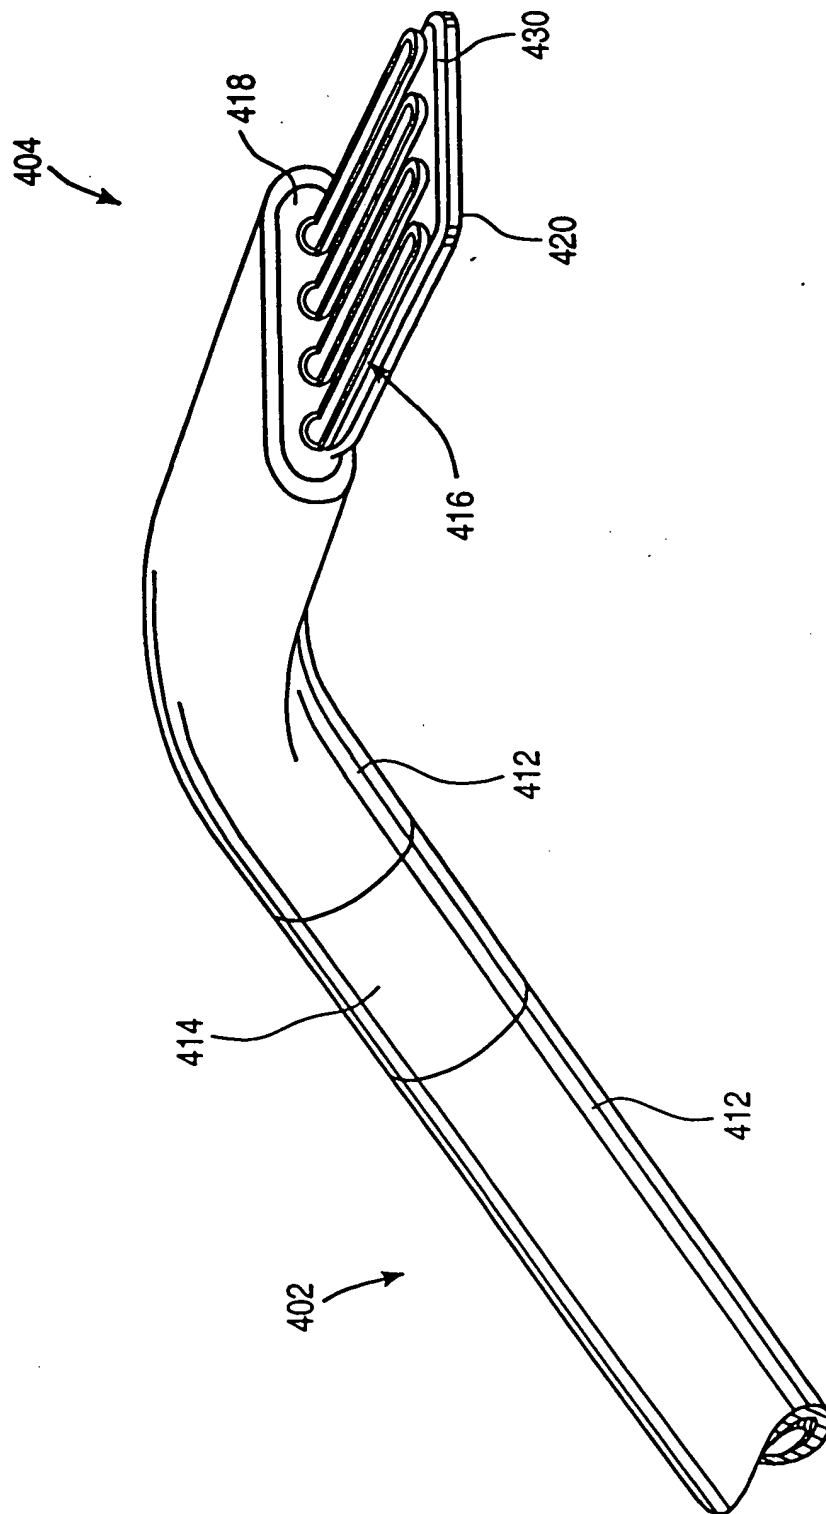


FIG. 21

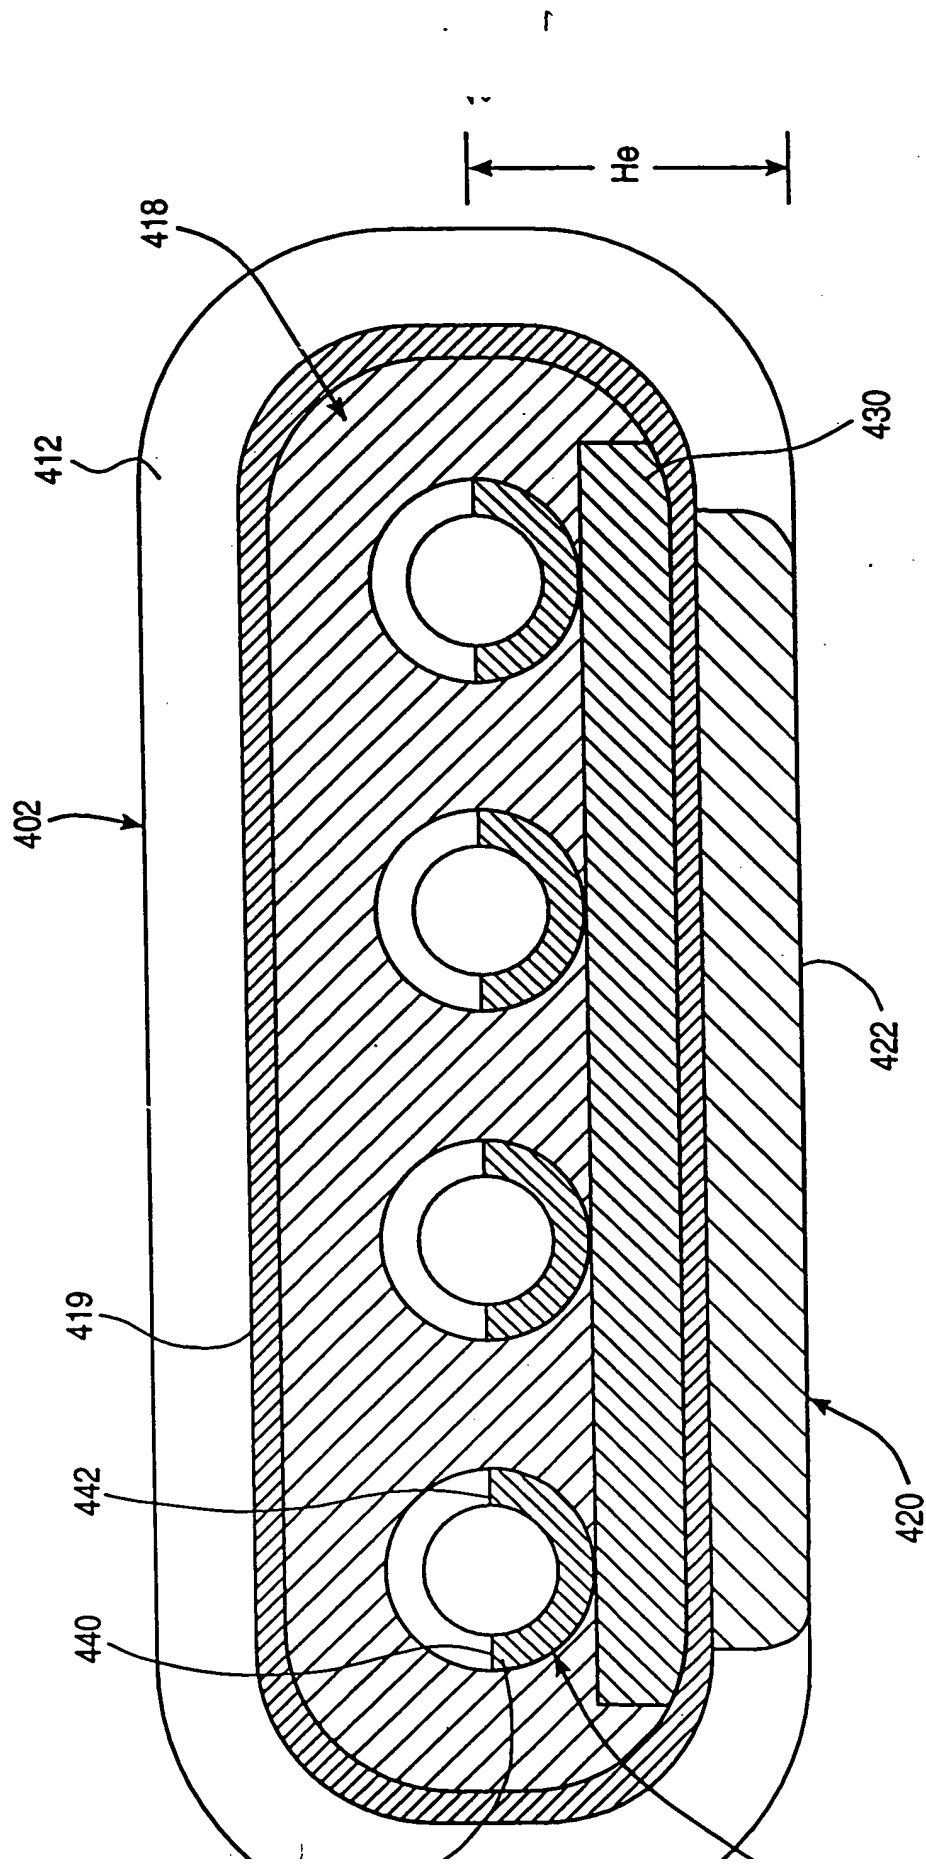


FIG. 22A

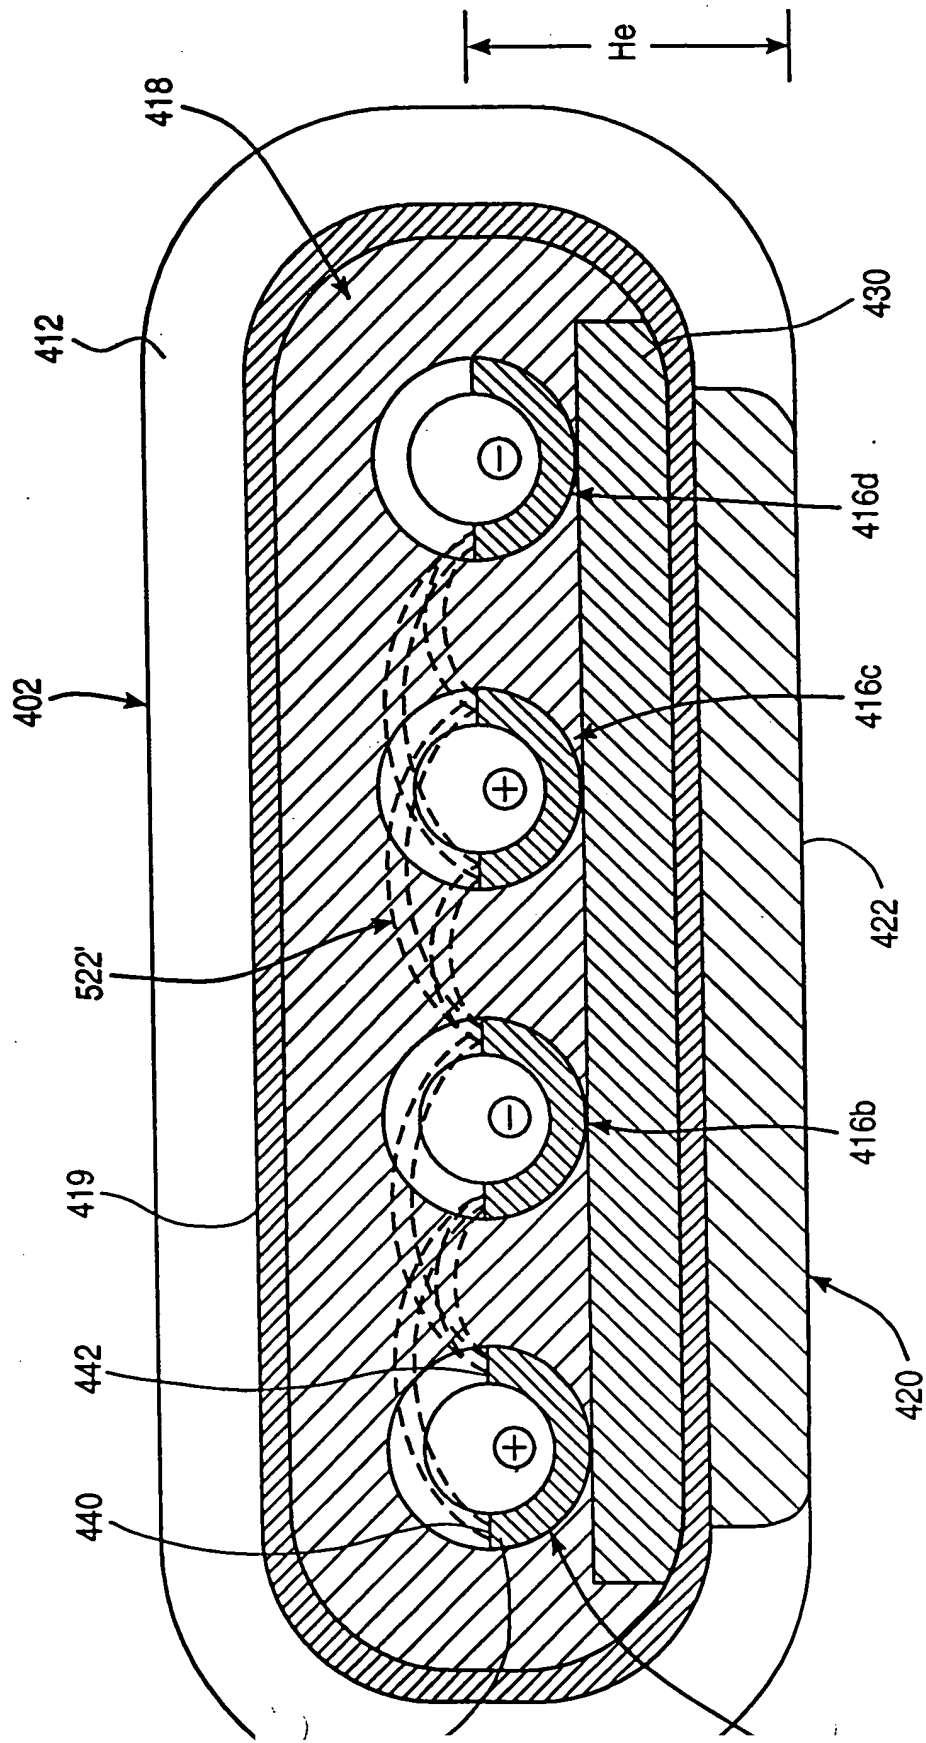


FIG. 22B

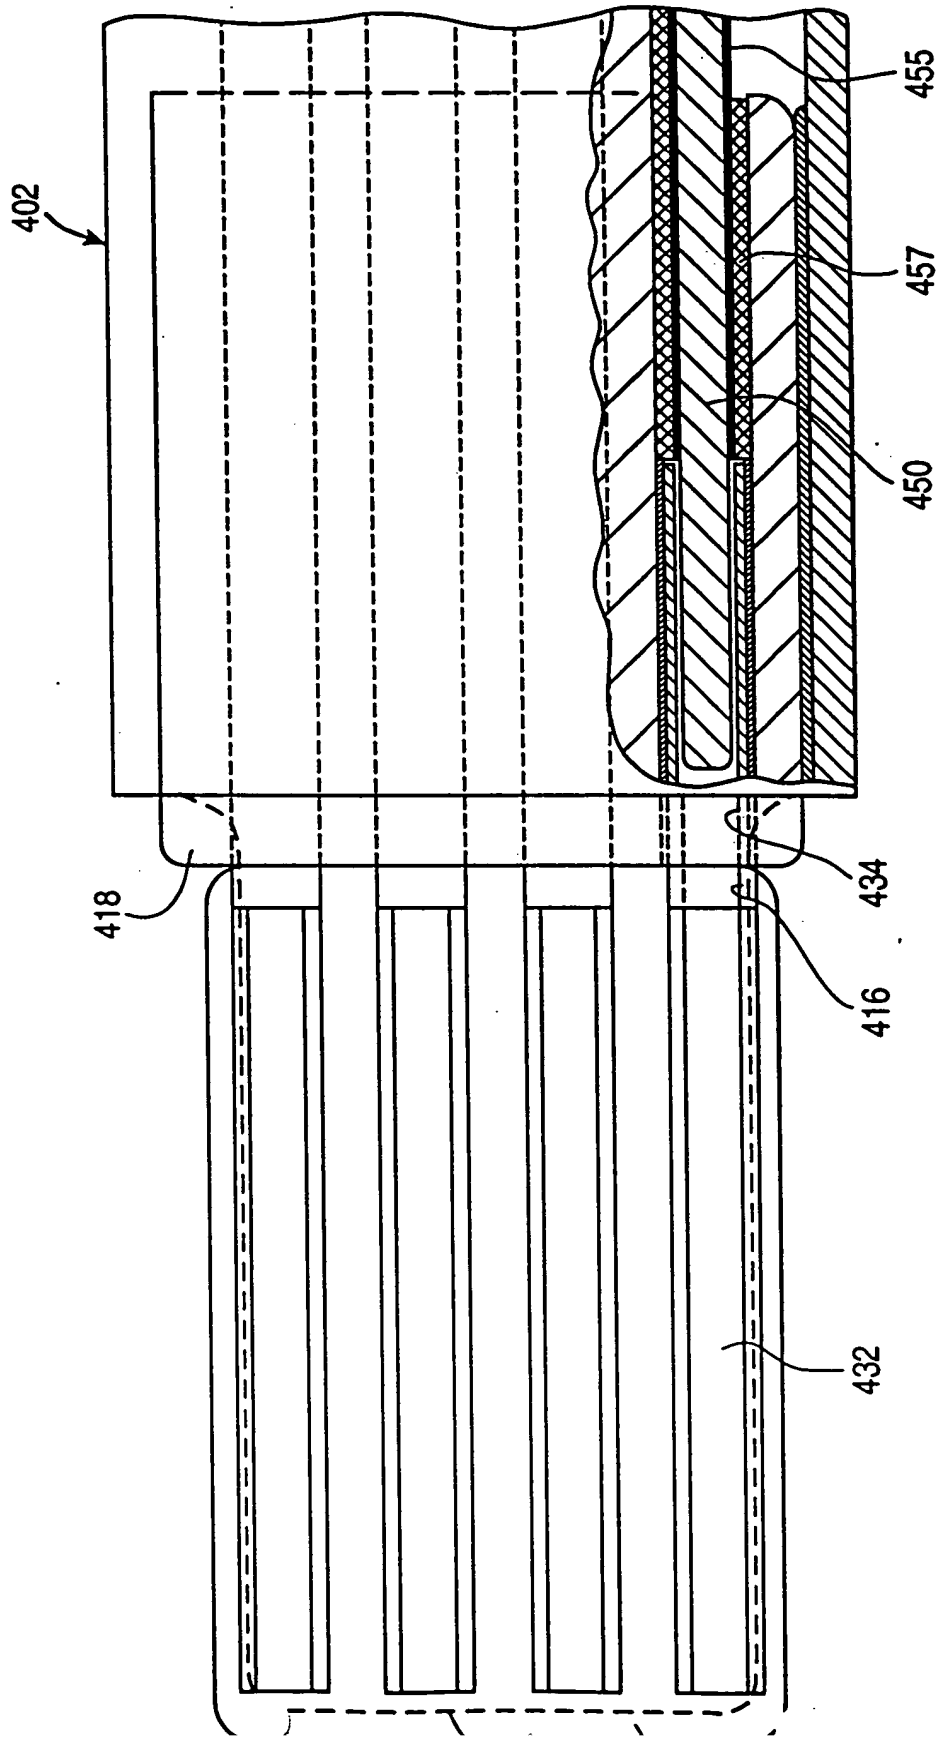


FIG. 22

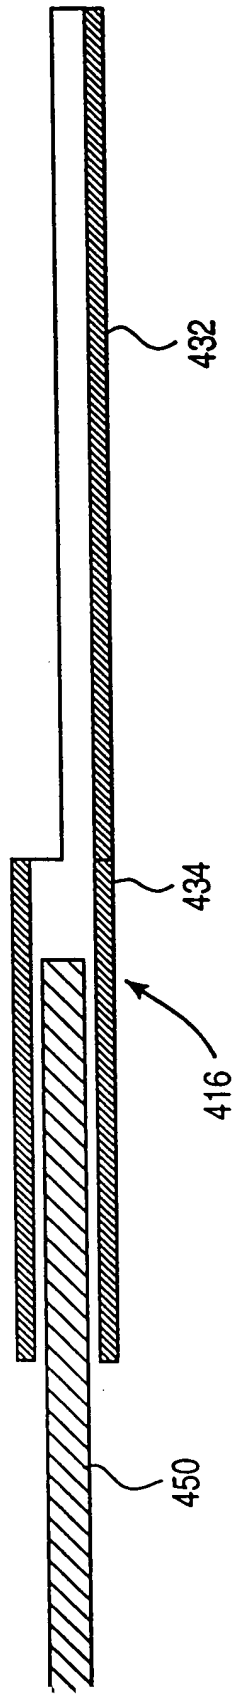


FIG. 23

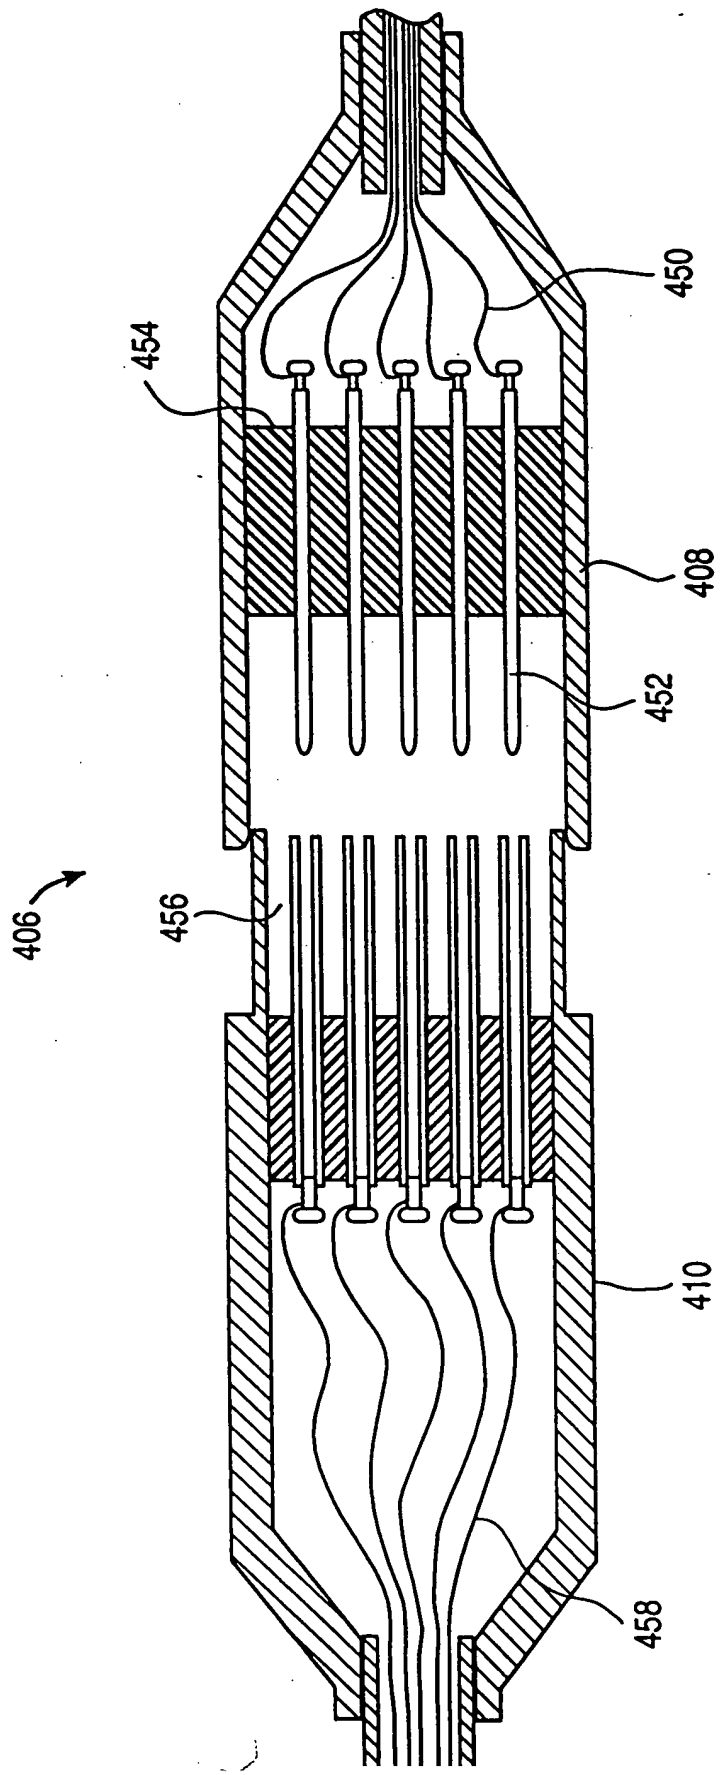


FIG. 24

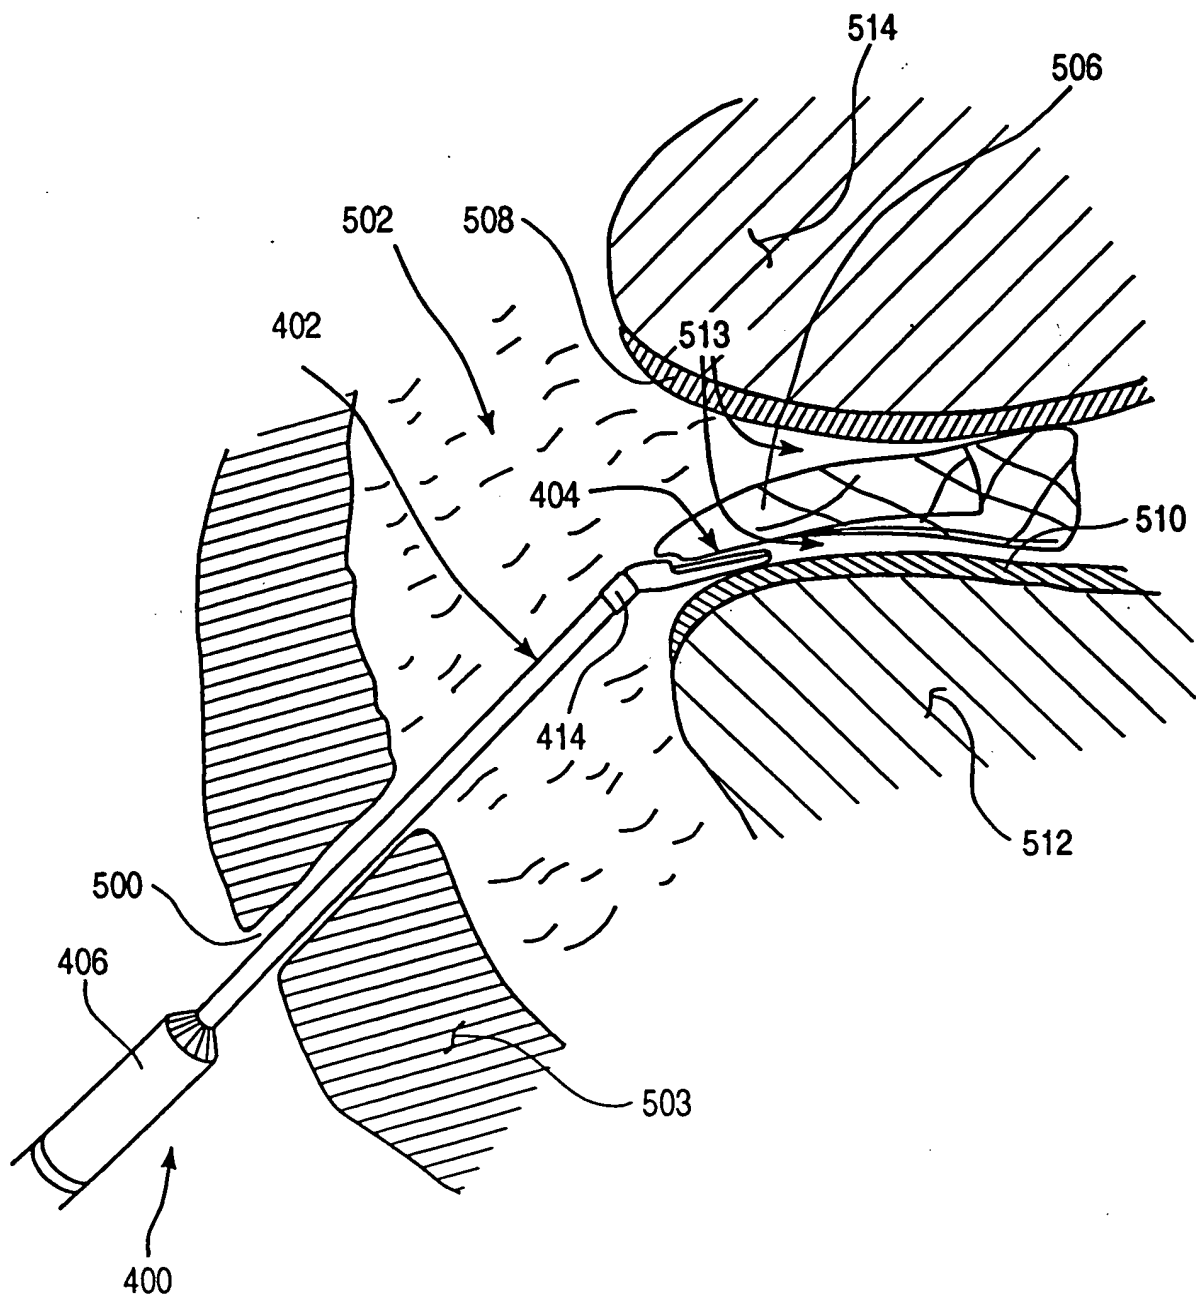


FIG. 25

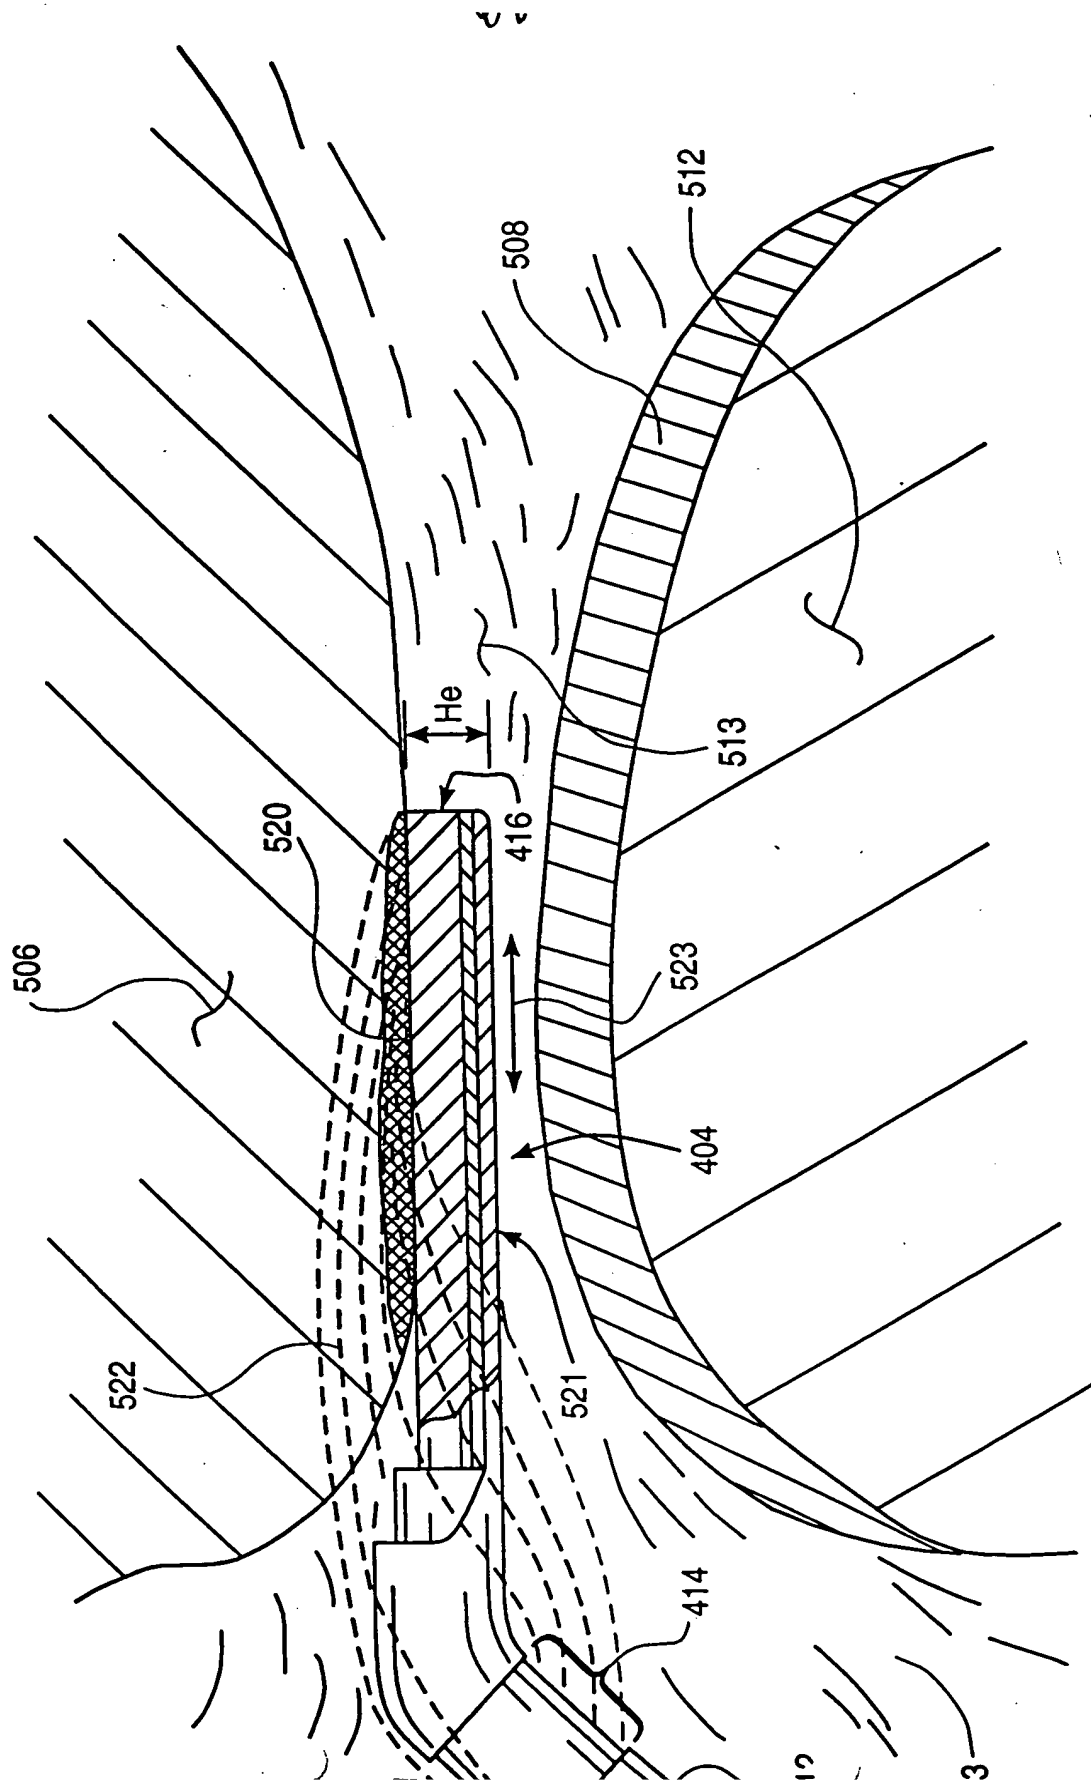


FIG. 2b

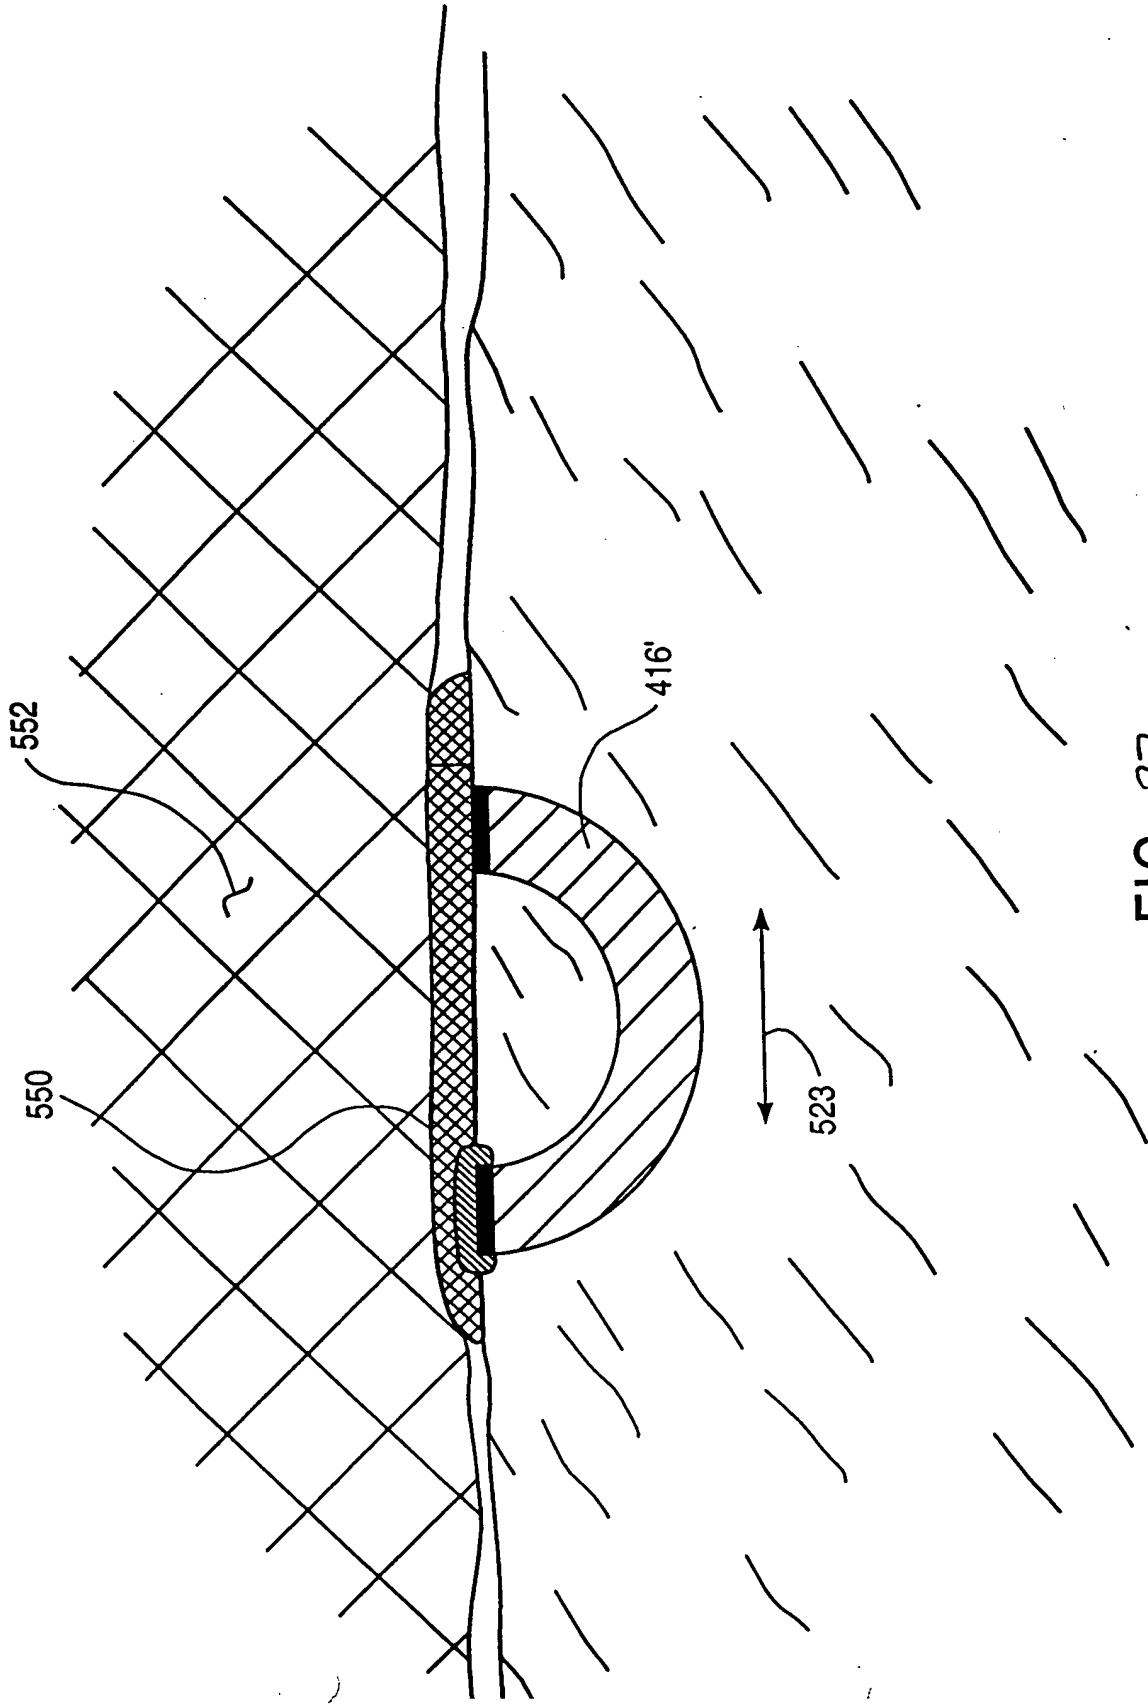


FIG. 27



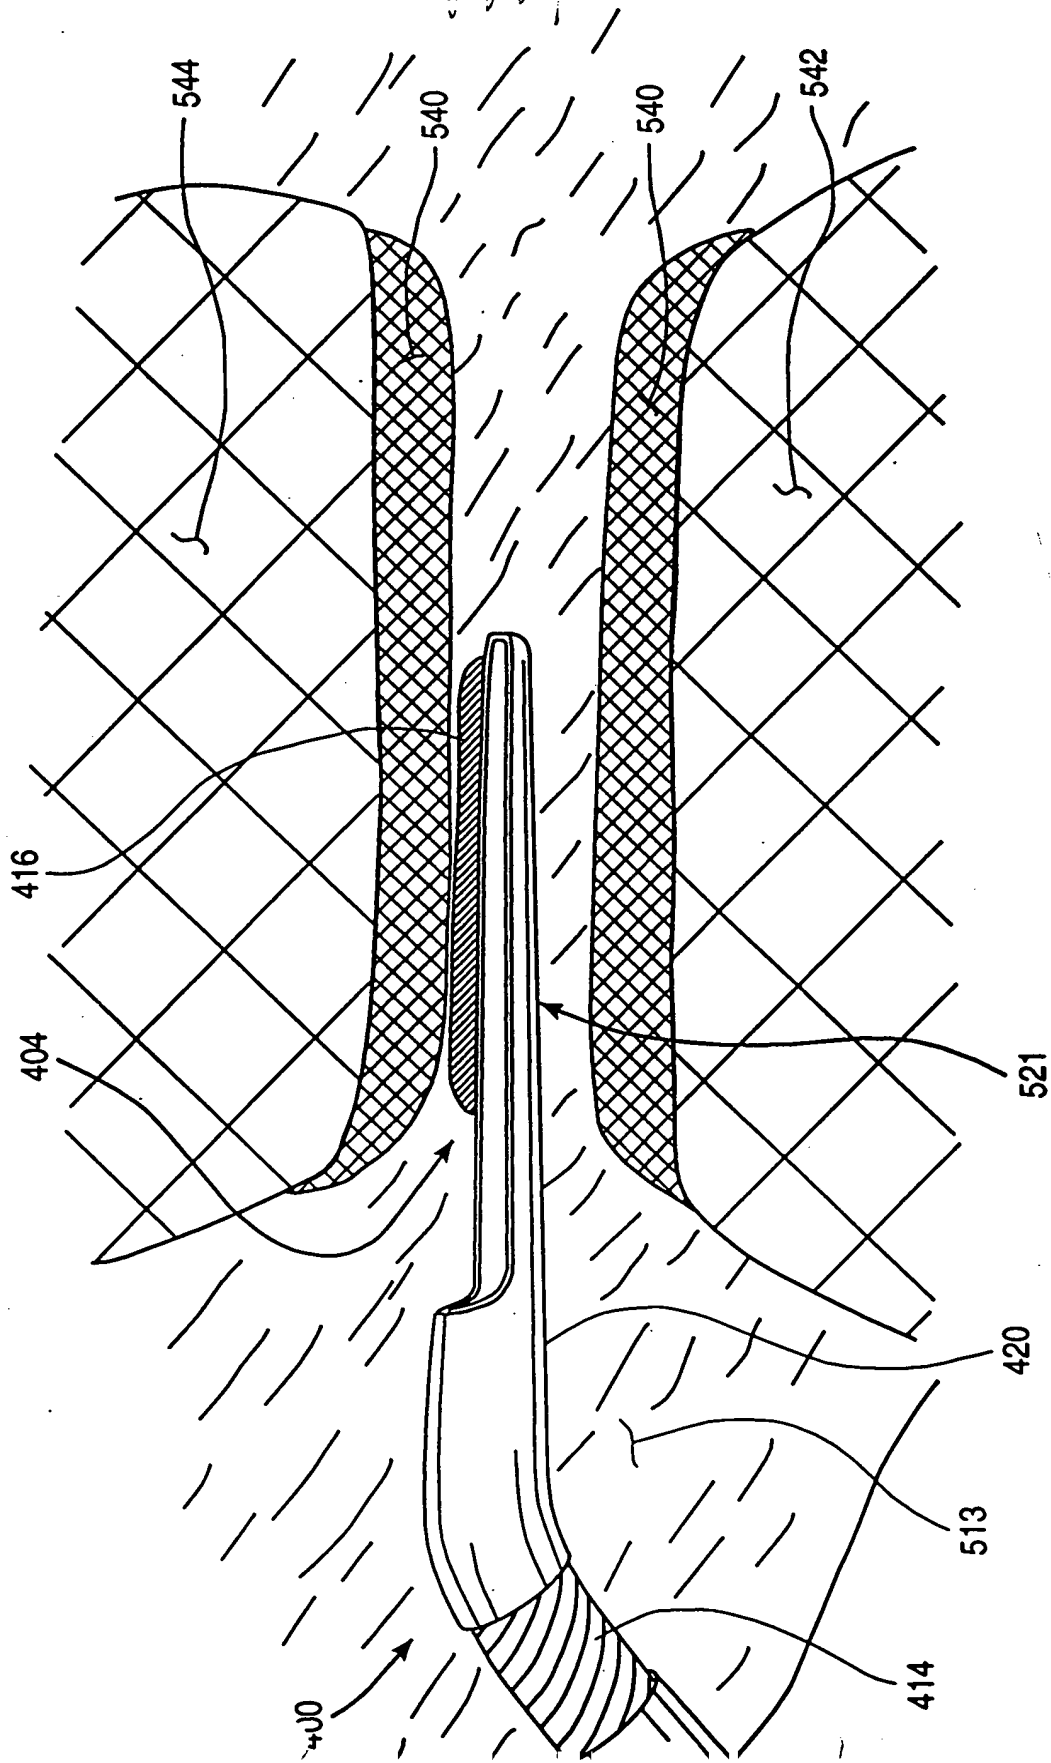


FIG. 28

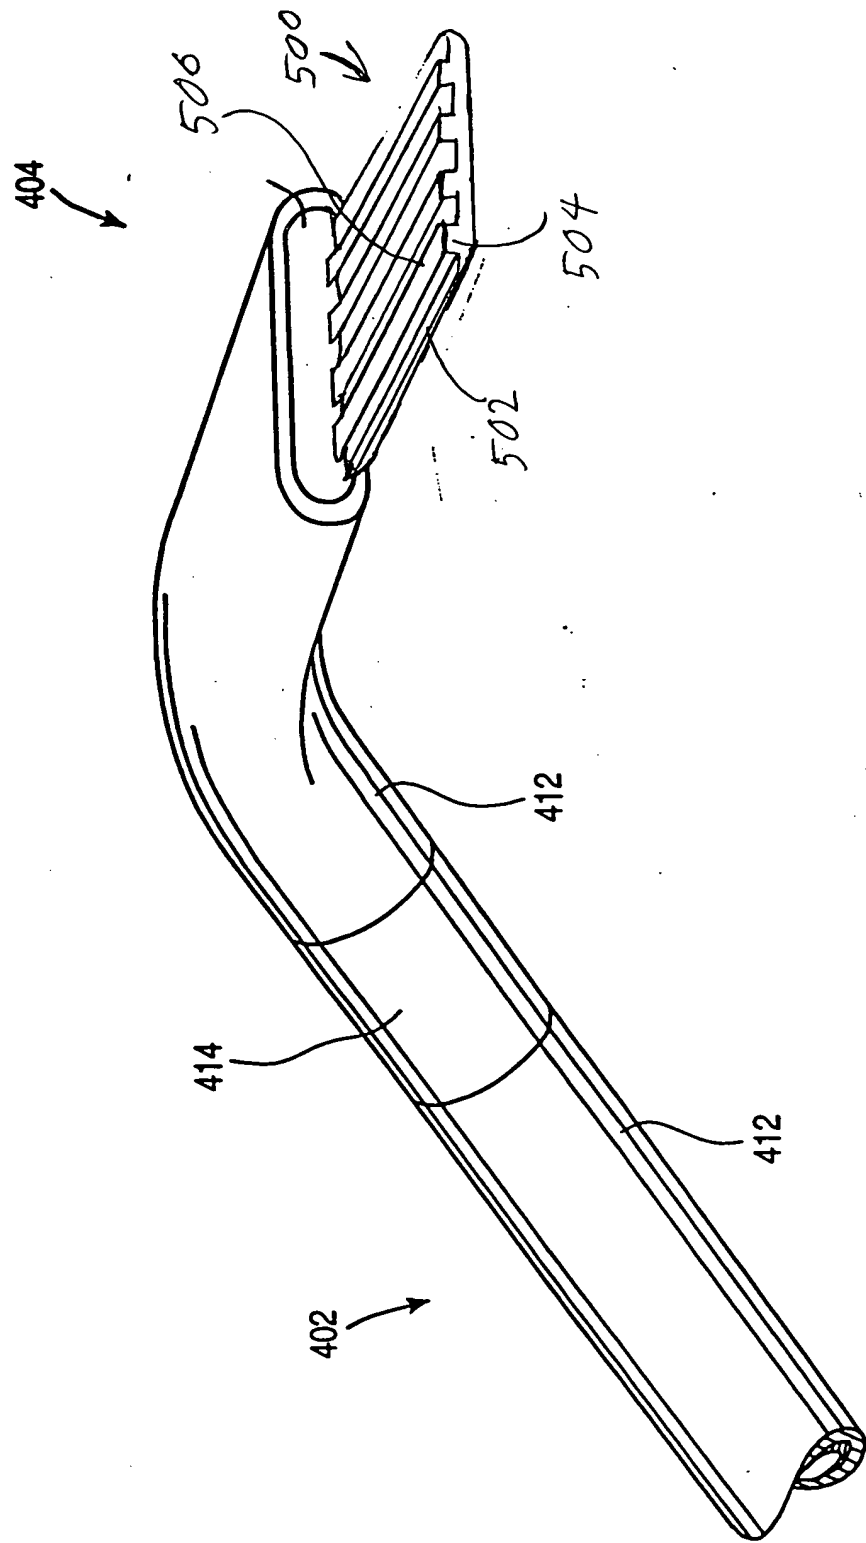

F1629

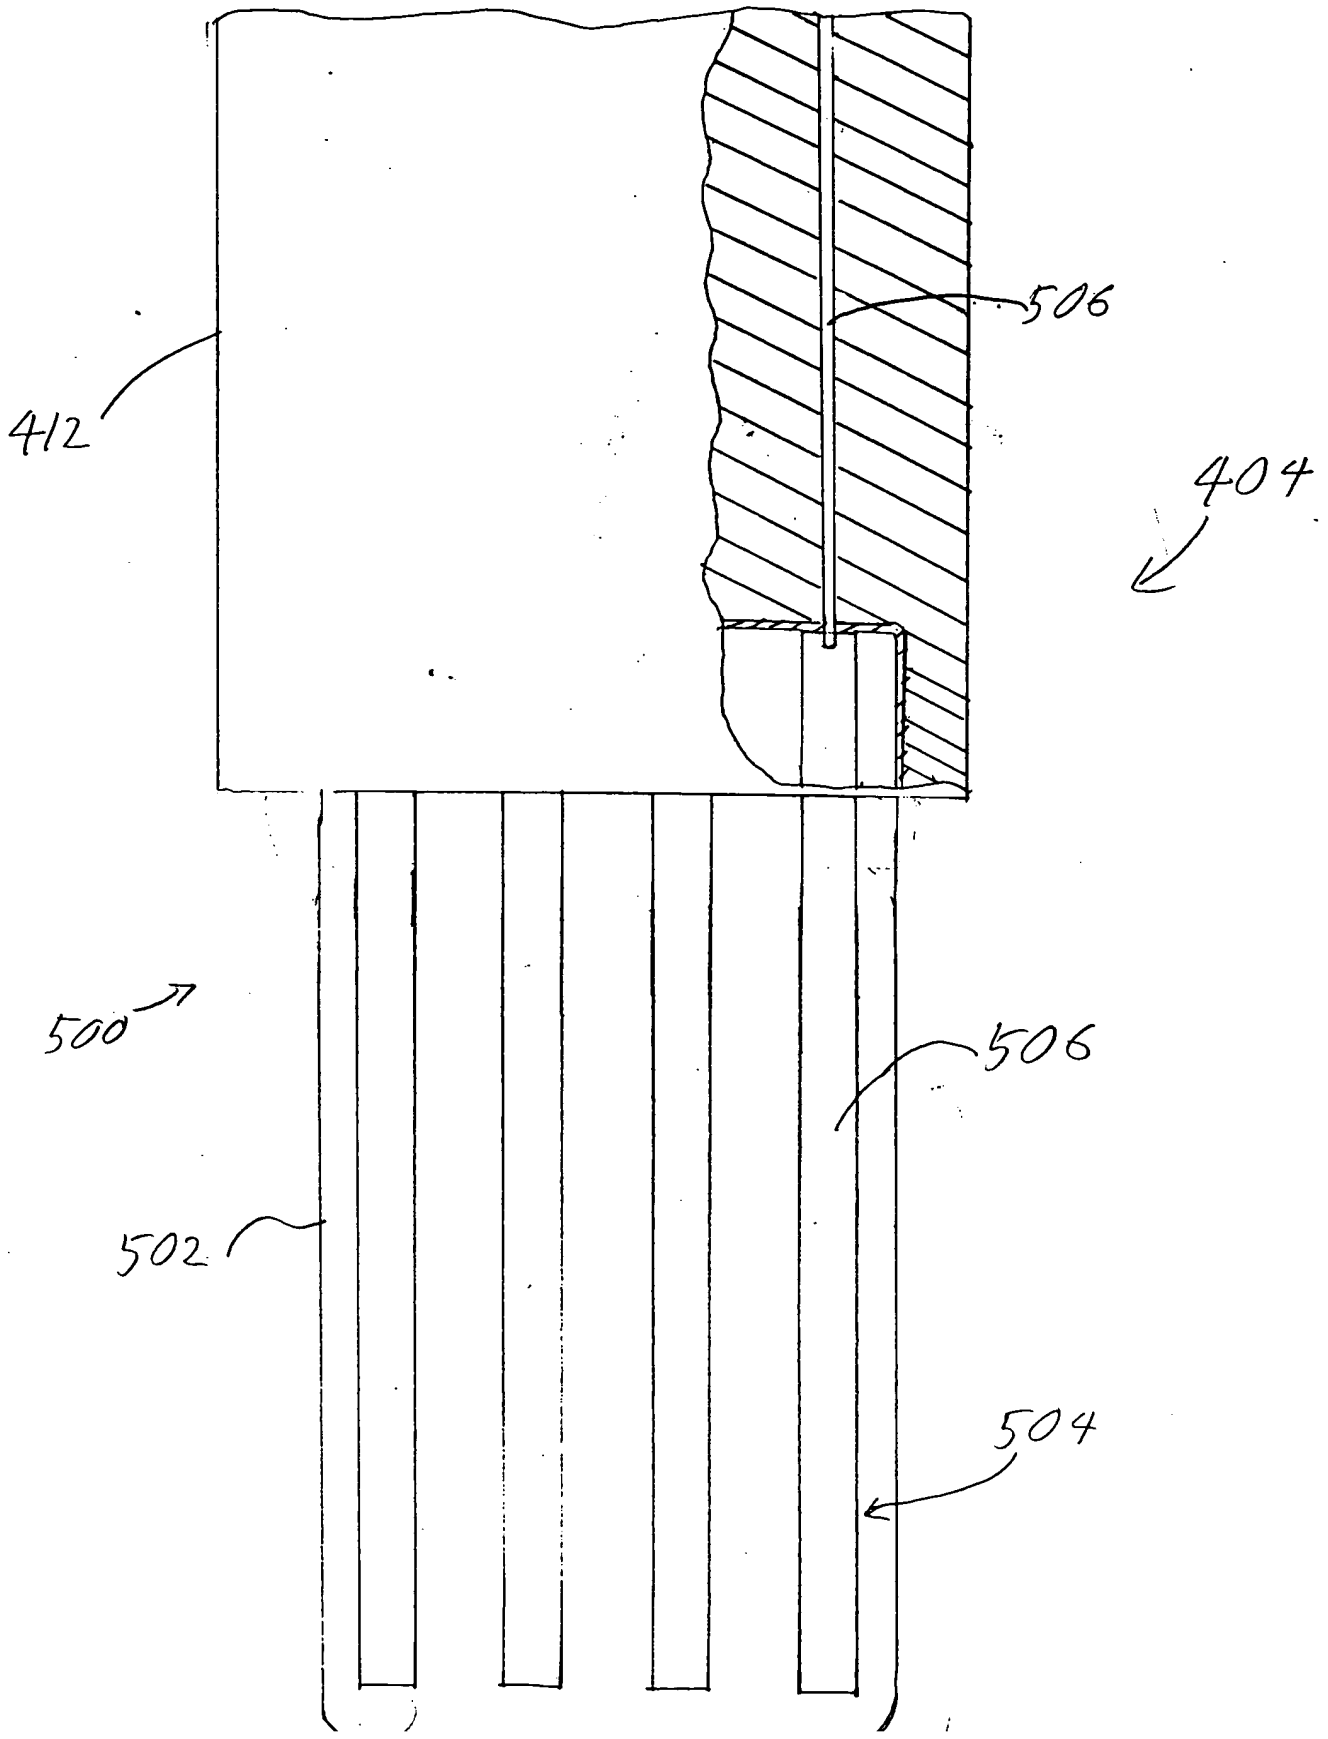

404

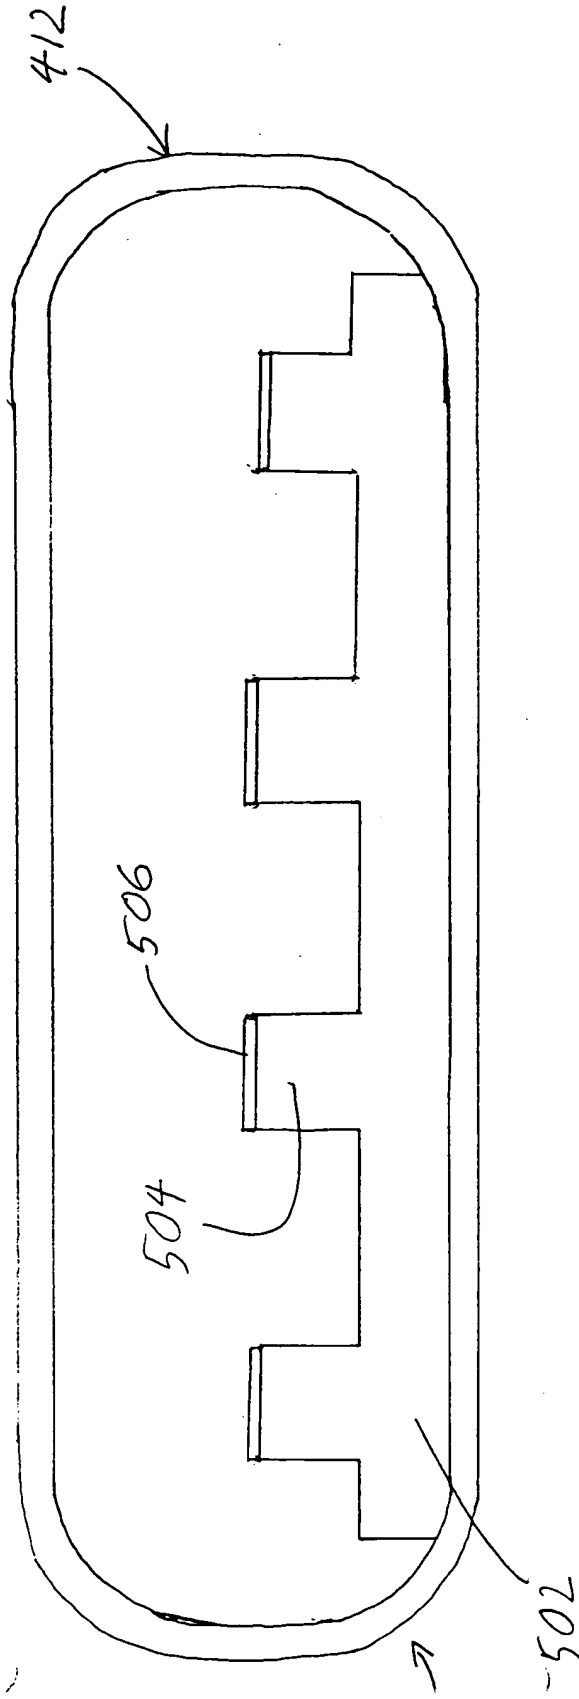


FIG. 31

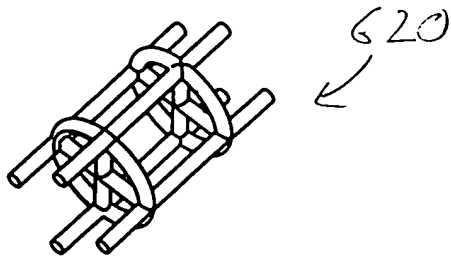


FIG. 32A




FIG. 32B

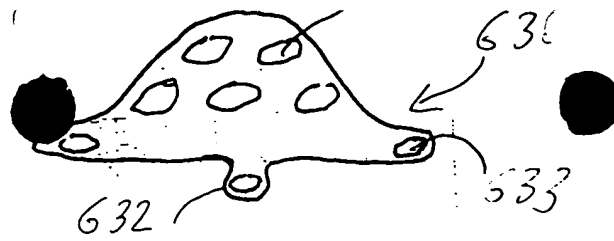


FIG. 33.A

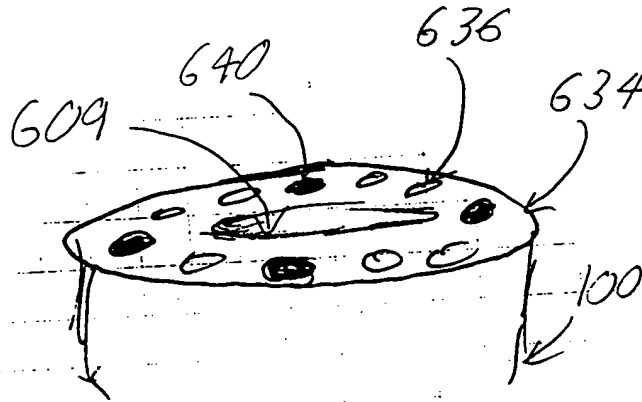


FIG. 33.B

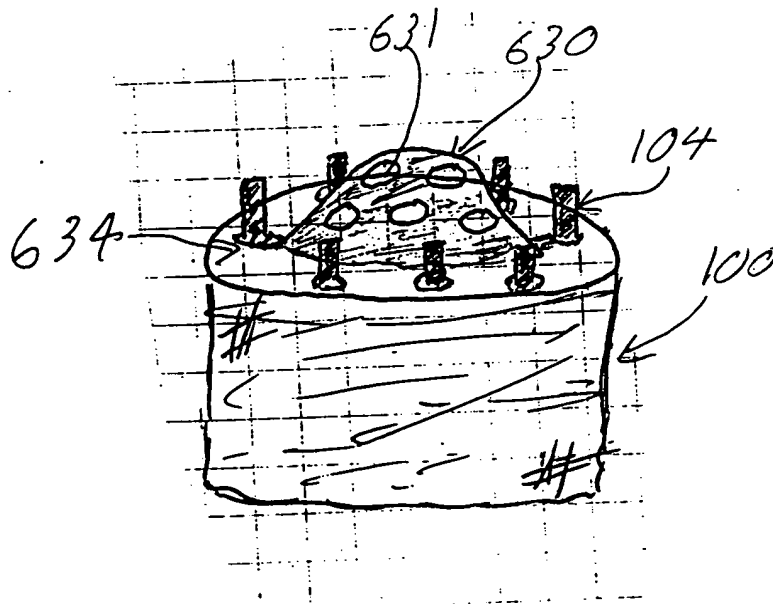


FIG. 33.C

FIG. 7 is a cross-sectional view of a medical device 700 inserted into a body cavity. The device 700 has a shaft 702 and a distal tip 704. A balloon 706 is inflated around the tip. A catheter 710 is also shown. Labels 720, 740, 760, and 780 indicate various anatomical or device components.

FIG. 34.

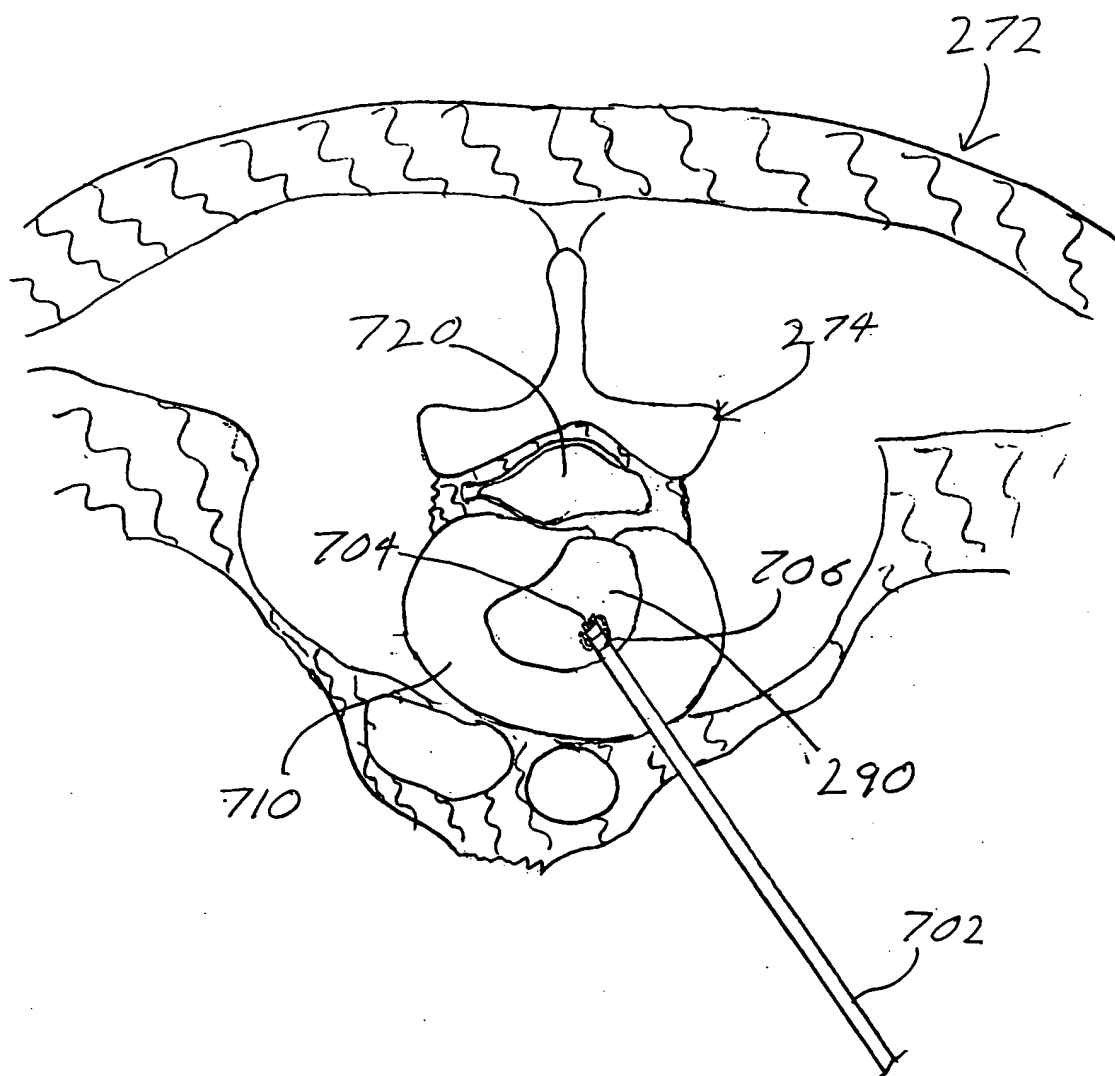


FIG. 35

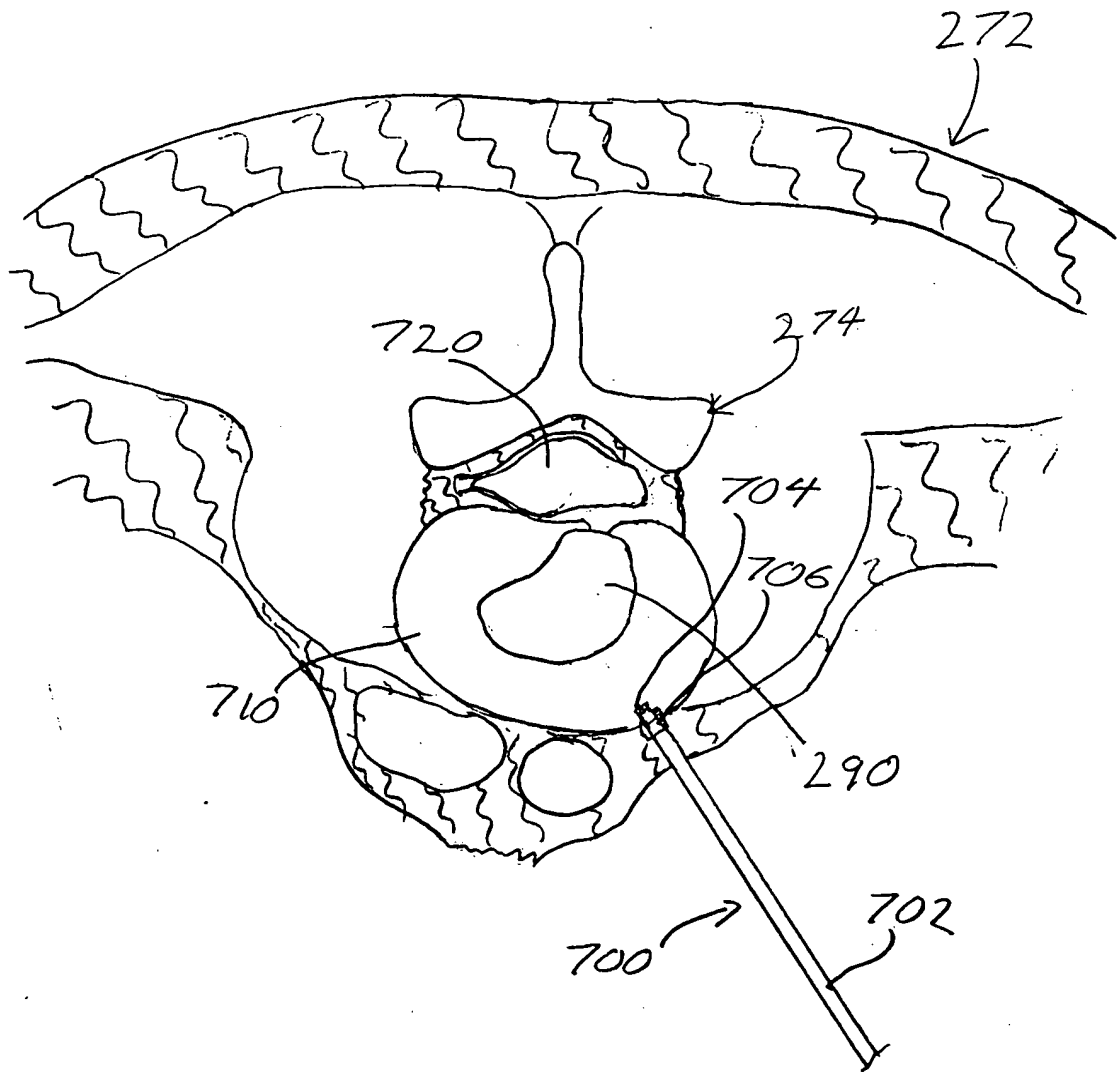


FIG. 36